

Shimadzu Electronic Balances General Catalog





Shimadzu began manufacturing balances in 1918. For more than 100 years, we have been at the forefront of providing precision, quality solutions for the most challenging R&D and QA/QC requirements. Our steadfast customer-focused commitment and unwavering dedication to technical excellence are both hallmarks of our history and the principles that guide us into the future.

Supporting manufacturing in the future, utilizing 100 years of experience and knowledge

SHIMADZU ELECTRONIC BALANCES

A Tradition of Weighing Expertise

Established in 1875 in Kyoto, Japan, Shimadzu Corporation is one of the pioneers of scientific precision instruments.

Top-pan and torsion balance production started in 1918, and equal-beam analytical balances were introduced in 1925. Since their release, the continuous improvement of Shimadzu balances has contributed to research and development across all industries.

Around the turn of the 20th century, precision weighing was a time-consuming practice performed only by experienced operators. Placing the sample and small masses on pans hung from a beam scale with a moving indicator was a tedious process. Shimadzu strove continuously to streamline weighing procedures. The introduction of the direct reading analytical balance (patented in Japan in 1948) signified a new era in weighing technology. In the Type L balance, the sensitive mass-loading work was replaced by convenient dial operations. This reduced weighing time by 66% and, subsequently, reduced demand for conventional balances.

Shimadzu then added the top-loading direct reading balance with Roberval's mechanism in 1959. Until recently, many of these instruments were still utilized in modern laboratories.

Shimadzu continued to pioneer technologies, releasing its first

electronic balance in 1971—the Digibalance. This release marked a milestone in precision weighing, introducing simplicity and ease of use to analytical weighing.

Six years later (1977), the application of microprocessors in electronic balances further enhanced weighing performance. The compact ED Series provided substantial improvements in sensitivity, resolution, and stability.

More recently, Shimadzu has introduced user-friendly instruments and features to the market, such as:

temperature-based fully-automatic calibration in 1985, the first one-piece force cell (OPF, later renamed UniBloc™) in 1989, the high-sensitivity AEM-5200 Micro Balance in 1993, and the unique Windows® Direct feature perfectly suited for the computerized laboratory of the 21st Century.

Its most recent achievement is the AP Series, advanced performance balances featuring UniBloc and a high response speed, and which are applicable for a wide range of applications.

Moving forward, Shimadzu is committed to providing innovative products for the analytical marketplace.

Contents

P 04 - UniBloc P 28 - Analytical Balances P 48 - Electronic Printers P 06 - Diverse Range of Functions P 34 - Electronic Balances P 49 - Specific Gravity Analyzers **Excellent Performance for** P 08 -P 40 - Top-Loading Balances P 54 - Animal Balances Multiple Industries P 10 - Product Lineup P 41 - Portable Flectronic Balances P 56 - Analytical Network Data System P 14 - AP Series P 42 - Precision Platform Balances P 58 - Optional Accessories P 26 - Static Remover (Ionizer) P 43 - Moisture Analyzers P 60 - Physical Dimensions



UniBloc Power!

Shimadzu balances advance to the UniBloc generation





Impact resistance test for four balances made by typical manufacturers. (Shimadzu internal test)

Test results of impact resistance test with top-loading balances (Minimum display: 10 mg)

Test conditions Free-falling the weight (3 kg) at 4 sec intervals.

(Weight was dropped 100,000 times from a height of 5 mm. After the first 100,000 tests, it was dropped from a height of 10 mm.)



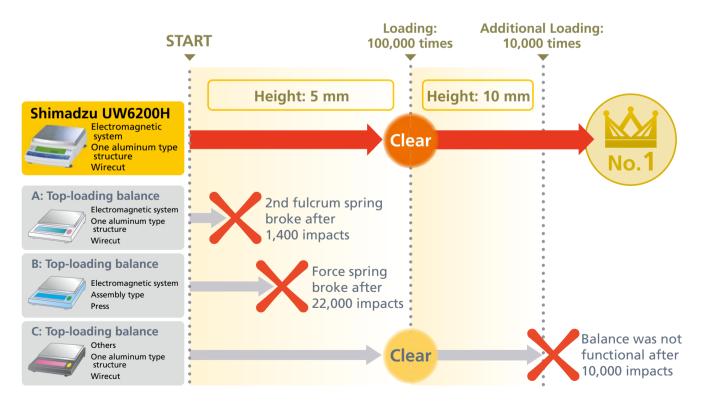

The results of this impact resistance test prove Shimadzu UW/UX series balances with UniBloc technology are the toughest. Put Shimadzu balances in your lab and experience UniBloc power.

UniBloc technology leads to a new era of measurement





Shimadzu introduced one-piece force cell technology for precision balances in 1989. Today's UniBloc is created by high-precision electric discharge wire processing applied to a block of aluminum alloy, and replaces the conventional electro-magnetic balance sensor assembly. UniBloc's compact, uniform structure ensures stable temperature characteristics, excellent response time and stable corner-load performance.

In addition, the UniBloc design permits a consistency of production that assures reliability and a long operational life.

The updated UniBloc technology expands the UniBloc balance lineup, which now ranges from semi-micro with a minimum display of 0.01 mg to precision platform balances up to 52 kg in capacity.

One-piece force cell patented in USA in 1989, No. 4799561, in China in 1991, No. 12729, in Japan in 1995, No. 1905686

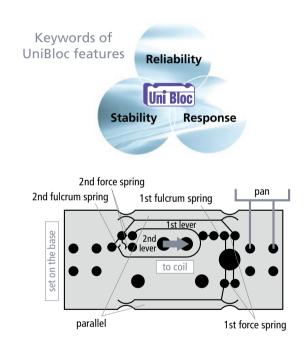

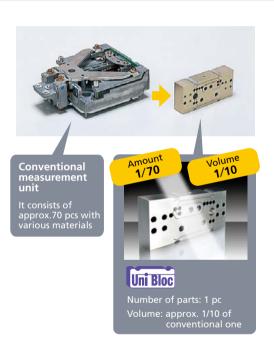



UniBloc family of balances


Shimadzu Balances Offer a Diverse Range of Functions

01

High Level Functionality

Rasy Setting

During operation, if you want to make the display slightly more stable, or alternatively, want to improve the response speed, you can make one-touch adjustments without interrupting measurement. A special indicator is provided that instantly shows the adjustment status.



Menu Operation Key

Easy-to-Operate Key Layout


Keys exclusively for menu operations are arranged separately from the measurement keys. Menus can be operated intuitively using the cross-shaped key layout.



Perfect Self Calibration

Electronic balances are precision instruments very susceptible to changes in room temperature. Sensitivity must be calibrated every time the balance is used since changes in room temperature influence mass measurement values, which are not supposed to change. The balance detects changes in room temperature that affect sensitivity, and automatically starts calibration using built-in weights. As a result, sensitivity errors are always kept within a constant range.

This allows the operator to concentrate on measurement tasks without having to worry about sensitivity calibration.




The perfect self calibration (PSC) function keeps the sensitivity error within a constant range at all times.

Clock-CAL

The balance starts calibration using built-in weights at preset times. If you set calibration times before important measurements (e.g. before starting work in the morning or during the lunch or evening break), the balance will automatically start calibration when the preset time is reached. This lets you

take stable, reliable measurements without worrying about sensitivity calibration.



02

Durability

Uni Bloc

Next-Generation Mass Sensor: UniBloc

Developed by Shimadzu, UniBloc is created by high-precision electric discharge wire processing applied to a block of aluminum alloy in order to replace the conventional sensor block assembly. As such, it uses no springs or screws. This uniform structure dramatically improves response and temperature characteristics, and the simple yet compact design enhances impact resistance. Balances equipped with UniBloc provide highly reliable mass measurement even during prolonged use.



03

Convenient Functions

Internal Calibration

The balance has built-in motor-driven calibration weights.

Sensitivity can be calibrated whenever needed with a single key press.

Single-Lever CAL

The balance has built-in calibration weights. Sensitivity is calibrated with a simple lever operation. Sensitivity can be calibrated easily, whenever needed.

Dry Battery Operation

The balance can also run on dry cell batteries, enabling use outdoors where no power is available.



Checkweighing

Preset the upper and lower limit values to display pass, high or low, depending on the sample weight.

Gomparator Output

Proper weight, high, low and other pass/fail judgments can be indicated by a buzzer, or output externally as a contact signal. (Optional comparator buzzer or relay output interface required.)

Backlight

Naturally, weight measurements can be taken even if the work site is dark, and prolonged use at normal work sites will not tire your eves.



GLP GMP

Built-in Clock

With the optional printer connected, data can be recorded with date and time stamps. Calibration reports can also be date- and time-stamped, which is ideal for establishing the measurement management and traceability required by GLP, GMP and ISO 9001.

ISO Calibration Report

Simply connect an optional printer to automatically print out which balance was calibrated when, and the calibration results. Absolutely no troublesome settings are required. Furthermore, the current date and time can be printed at any time during measurement.



(AUW Series Printout Sample)

PC Connection

Balance Keys

Using Balance Keys, a balance data collection software, allows importing balance data directly to a user's applications with the intuitive feel of keyboard input. In addition, data from multiple balances can be imported.

RS-232C Interface

Equipped with an RS-232C interface for easy integration with other devices and computers.

Computer Connection Function

Systems can be connected to a computer via an optional cable/adapter kit. For more details, visit the Shimadzu website.

Network



LabSolutions™ Balance

Connecting with LabSolutions lets you save data from balances, HPLC and other analytical instruments to a database, and create reports automatically. Uniform data management means no transcription errors and is perfect for security.



Applications

Piece Counting

A built-in piece counting function enables balances to be used as parts counters (piece scales).



Specific Gravity Measurement

A specific gravity calculation function based on the immersion method is built in.

Just attach the optional Specific Gravity Measurement Kit to use a balance as a specific gravity meter.



Built-in Animal Measurement Mode

The weight of mice, rats, rabbits, and other small animals can be measured. Stable measurements are obtained even if the animal moves.





Results can be displayed in carats when measuring precious stones.



Excellent Performance for Multiple Industries



- Weigh liquids and powders in development departments
- Measure specific gravity and moisture ratio of resin pellets, rubber, etc.
- Input mass values via connection to a titration system for quality management
- Measure mass and moisture ratio of dyes, pigments, and inks
- Measure and control materials accumulated on filters
- Control moisture ratio levels during catalyst production
- Check weights when receiving raw materials
- Confirm the net weight of final products
- Measure the moisture ratio and control the quality of raw materials and products
- Weigh trace quantities of additives
- Weigh raw materials during formulation





- Control pharmaceutical usage quantities by measuring weight before and after use
- Weigh raw materials
- Confirm the weight of stents and other miniature medical devices
- Measure the moisture ratio and control the quality of raw materials and products
- Measure weight changes during animal experiments
- Measure drugs during drug manufacturing processes
- Measure weight changes in creams and compresses at specified intervals
- Control the quality of product containers and cases
- Measure the moisture ratio of hair, etc.






- Count the number of very small products
- Check the weight of coated steel sheets/plates after polishing
- Control the moisture ratio and specific gravity of iron and steel raw materials
- Measure trace quantities machined from metals, etc.
- Measure the specific gravity of rare metals and compare it to theoretical values
- Control the amount of wear on metal materials
- Weigh items when purchasing precious metals or bullion

Electronics

- Check weights when manufacturing electronic circuit boards
- Measure tiny semiconductor parts
- Check for missing items in product packages based on weight
- Control the quantity of plastics used in LED lenses






- Measure electrolyte injection quantities on lithium-ion battery production lines
- Measure moisture ratio in sheet materials
- Control contamination remaining on machinery parts


- Use for training students
- Manage reagent use by weight, in combination with a chemical substances management system
- Use in lectures to explain basic principles and theory









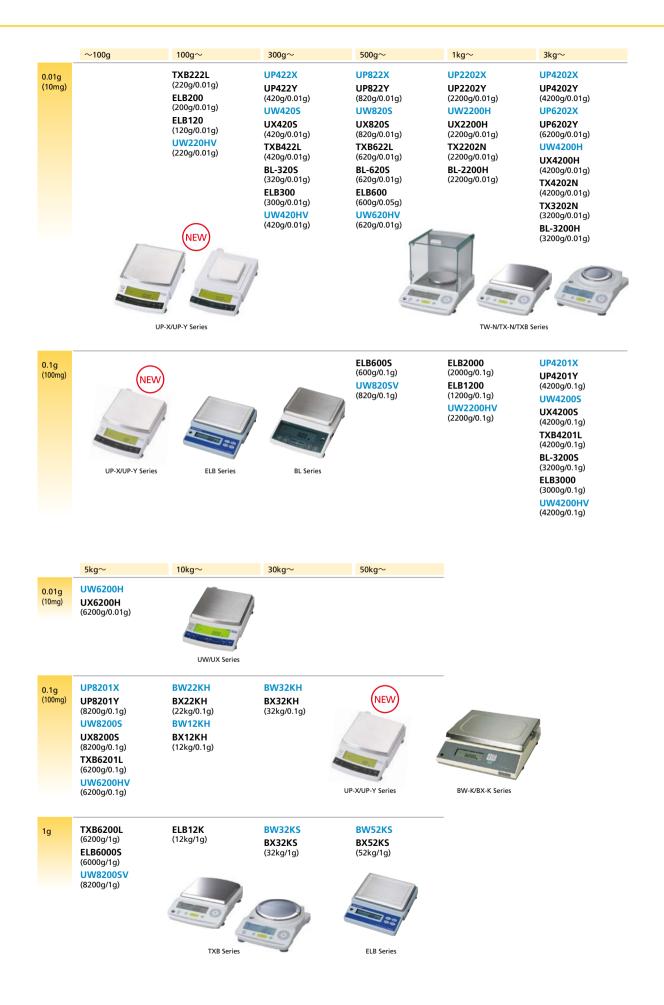



 \bigcirc : Standard function \triangle : Option

○ : Standa	○: Standard function △: Option								
		AP-WD AP-W	AP-X	AP-Y	AUW-D AUW	AUX	AUY	ATX-R ATY-R	ATX ATY
Uni Bloc	UniBloc	0	0	0	0	0	0	0	0
PSC	Perfect Self Calibration	0	0		0	0		(ATX-R only)	
Clock CAL	Clock-CAL	0	0		0			, ,,	
Thm Motor-CAL	Internal Calibration	0	0		0	0		(ATX-R only)	(ATX only)
Ž	Single-Lever CAL								
Built-in	Built-in Clock	0	0	0	0	0			
iso	ISO Calibration Report	0	0	0	0	0			
	Menu Operation Key	0	0	0					
XY.	Easy Setting	0	0	0				0	0
Back Light	Backlight				(AUW only)				
000	Organic EL Display	0	0	0					
PC	Computer Connection Function	0	0	0	0	0	0	0	△*1
Balance Keys	Balance Keys	0	0	0	0	0	0	0	0
RS-232C INTERFACE	Built-in RS-232C Interface	0	0	0	0	0	0	0	△*1
USB INTERFACE	Built-in USB Interface	0	0	0				0	
Analog display	Analog Bar Graphic Display	0	0	0	0	0	0		
H I G O L O	Checkweighing	0	0	0				0	\circ
1	Comparator Output								
PCS	Piece Counting	0	0	0	0	0	0	0	0
CARAT	Carat Measurement	0	0	0	0	0	0	0	0
Specific Gravity	Specific Gravity Measurement	0	0	0	0	0	0	0	
D RY Battery	Dry Battery Operation								
[5]	Standard Below-weigh Hook	0	0	0	0	0	0		
	Built-in Animal Measurement Mode								
12	Formulation Mode	0	0	0	0	0	0	0	0
	Internal Timer Output	0	0	0	0	0			

^{*1} Requires optional I/O–RS conversion cable or interface IFB-102A. *2 Requires an optional below-weigh hook. *3 The picture is UP-X. *4 The picture is UP-Y.



UP-X UW*3	UP-Y UX*4	TW TX	TXB	BW-K BX-K	ELB	BL	UW-V	MOC63u MOC-120H
0	0	0		0			0	0
0							0	
0							0	
0		(TW-N only)					0	
				(BW-K only)				
0	0			0			0	0
0	0			0			0	0
		0	0					
		0	0					
0	0	0	0				0	0
		_	_	_				
0	0	0	0	0	△*1	△*1	0	0
0	0	0	0	0	0	0	0	0
0	0	0	0	0	△*1	△*1	0	0
				0				(MOC63u only)
0	0	0	0	0		0	0	
0							0	
0	0	0	0	0	0	0	0	
0	0	0	0	0		0	0	
0	0			0	0		0	
Ų.			0		0		Ű	
0	0			△*2	△*²		0	
0	0			0	_		ÿ	
0	0	0	0	0			0	
0				0				0
0	0			0				0

AP Series



Advanced Performance UniBloc Balances

Provides High-speed Response and High Stability A New Stage in Analytical Balance Performance

High Speed

This significantly improves weighing efficiency.

Stress Free

This eliminates the influence of static electricity, achieving reliable measurements in a simpler

For Regulation


Interlocking with LabSolutions Balance enables compliance with a variety of data integrity regulations, including ISO 17025 for testing laboratories, ISO 9001 and ISO 14001 for the manufacturing industry, and GLP/GMP and the United States Pharmacopeia (USP) for the pharmaceutical industry.

Functions are included for the preparation of buffer solutions used in HPLC. As a result, the operation can be performed accurately and easily, even by non-specialists.

Save Your Operation

Equipped with USB as standard*1. Includes many diverse functions to support users.

^{*1} All models: USB-B type connector as standard AP-W Series: USB-A type and B type as standard







Watch the AP overview video on our website.

https://www.shimadzu.com/an/balance/analytical/ap.html

Series

High Speed

Fast measurement significantly improves operational efficiency.

Fast Response with UniBloc AP Technology


Shimadzu analytical balances boast the one-piece UniBloc weighing sensor, which is now even more advanced.

The response time is reduced to about 1/5 the time of previous models. In addition, the UniBloc sensor offers a response time of just 2 seconds, an improvement from 10 seconds with the previous model.

Response During Trace Measurements with the 0.01 mg Model (Equivalent to 1 mg / With Conditions Set by Shimadzu)



Response During Trace Measurements with the 0.1 mg Model (Equivalent to 1 mg / With Conditions Set by Shimadzu)




Model	Previous Model	AP Series
0.01 mg	10 sec.	2 sec.
0.1 mg	7 sec.	1.5 sec.



Built-in High-Performance Ionizer (Optional)

Comparison of Neutralization Speed (Representative Values)

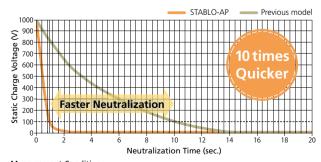


Measurement Conditions

- Time from ±1000 V to ±100 V
- For this evaluation, a 150 × 150 mm charged plate monitor (CPM, 20pF) was used.
- Distance between CPM and ionizer: 100 mm

The ionizer eliminates influence of static electricity in 1/10 the time of previous models.

Note: Example of typical static electricity removal time ($\pm 1000 \text{ V} \rightarrow \pm 100 \text{ V}$) 1 sec. for STABLO-AP and 10 sec. for STABLO-EX (previous model)



AC Method with



Stress Free

A variety of accessories and options suitable for semi-micro measurements



Increased weighing capacity from 135 mg to 220 g (0.01 mg model)

Micro amount weighing over 135 mg (read 0.01 mg step) is possible.

Improved Sensitivity Stability When Ambient Temperature Changes

The temperature of the operational environment is affected by the external air temperature, turning off the air-conditioning, people entering the room, etc. The stability with respect to these small temperature variations in the operational environment has been improved. When the ambient temperature has changed by +1 °C in 20 minutes, the AP225W provides an improvement in the stability of the sensitivity by a factor of four compared to the previous model.

 Change in Sensitivity When Repeatedly Weighing 200 g (Measurement carried out by Shimadzu)

(When the ambient temperature has changed by +1 °C in 20 minutes)

Previous model

Time [min.]

Improved Minimum Weight

(Minimum display 0.01mg, AP225W/135W/225WD/125WD only)

By improving stability technologies, the minimum weight required for meeting USP Chapter 41 requirements has been improved from 30 mg to 20 mg.

The AP Holder (standard accessory for AP225W) compatible with a variety of weighing containers is provided standard, and static electricity is properly removed from the bottom of the container, resulting in easier operation.

→ The AP Holder in combination with the ionizer can eliminate the influence of static electricity on the weight value. See page 23 for more information.



Volumetric flask (100 mL)



Test tube (10 mL)



AP Holder

Containers that can be used with the AP Holder (Examples)

Container	Applicable Volume*	
Volumetric flask	10 to 100 mL	
Conical flask	100	
Beaker	100 mL	
Centrifuge tube (Spitz tube)	2 . 25	
Test tube	3 to 25 mL	

^{*} About 70 mm or more height or length is required.

Easy-to-Use Multi Stand

(0.01 mg model only, equipped as standard)



With weighing paper, for example, if the tare is larger than the pan diameter, measurements can be simplified by attaching the special multi stand.



The internal windbreak plate suppresses the influence of convection and air flow within the weighing chamber, improving the stability and response of measurement values.

Series

For HPLC

Buffer Solution Preparation Mode **NEW**

(AP-W Series only)

·Recipes for 13 commonly used buffer solutions are included

Preparation recipes for commonly used buffer solutions are provided as standard. e.g. disodium phosphate, sodium acid citrate

New buffer solution recipes can be registered

If a buffer solution is not registered by default, it can be added.

Instructions are shown on the display

The target weighing value is shown on the display and analog bar in order to compare the target with the current weight. Manual calculation is not needed.

Record function

Record output with date, time and operator name.

The pH level of mobile phase (eluent) solutions used in liquid chromatographs is adjusted to improve separation of components and extend the life of columns. This pH adjustment process is performed using a buffer solution. Currently, the most common method is using a pH meter to measure the pH as the solution is prepared; however, this process requires considerable time and effort, which can cause operational bottlenecks.

An alternative method does not require a pH meter. It involves preparing solutions by weighing fixed theoretically calculated quantities of an

AP series supports weighing these acids and bases. If the type and quantity of the buffer solution are specified, the balance displays the type and quantity of sample that should be weighed. Then the buffer solution can be prepared easily by adding water to the specified quantity of

Preparation example: When weighing and preparing 50 mM of di-sodium hydrogen phosphate, 2-hydrate and 50 mM of sodium dihydrogenphosphate, 2-hydrate in order to prepare 3 L of 100 mM phosphoric acid (sodium) buffer solution at pH = 2.1:

Example of preparation by AP series



solution

Number	Buffer solution preparation list			
1	100 mM	phosphoric acid (sodium)	pH = 2.1	
2	10 mM	phosphoric acid (sodium)	pH = 2.6	
3	50 mM	phosphoric acid (sodium)	pH = 2.8	
4	100 mM	phosphoric acid (sodium)	pH = 6.8	
5	10 mM	phosphoric acid (sodium)	pH = 6.9	
6	20 mM	citric acid (sodium)	pH = 3.1	
7	20 mM	citric acid (sodium)	pH = 4.6	
8	10 mM	tartaric acid (sodium)	pH = 2.9	
9	10 mM	tartaric acid (sodium)	pH = 4.2	
10	20 mM	acetic acid (ethanolamine)	pH = 9.6	
11	100 mM	acetic acid (sodium)	pH = 4.7	
12	100 mM	boric acid (potassium)	pH = 9.1	
13	100 mM	boric acid (sodium)	pH = 9.1	

^{*} Results can be printed with date/time and user ID

For Users of HPLC Systems

Sample Preparation NEW

(AP-W Series only)

When preparing a standard solution from a particular component, the standard powder for this component will be a hydrochloride or a hydrate. Preparing a standard solution of the target component at a desired concentration requires difficult calculations prior to weighing it. With the AP series, however, the required weight value is automatically calculated, so it can be weighed without performing manual calculations.

Example of preparation by AP series

Weigh 25 mg Amitriptyline to make a standard solution

Standard sample of Amitriptyline is Amitriptyline Hydrochloride.

Calculation is essential to determine part of Acidum hydrochloricum by molecular weight in order to make a 100 mg/mL Amitriptyline solution.

Molecular weight of Amitriptyline: 277.4

Molecular weight of Acidum hydrochloricum: 36.5

Molecular weight of Amitriptyline Hydrochloride: 277.4 + 36.5 = 313.9

To compare the molecular weight of Amitriptyline Hydrochloride with Amitriptyline, the following calculation is necessary.

313.9/277.4 = 1.132

The molecular weight of Amitriptyline Hydrochloride is 1.132 times of Amitriptyline.

So, if 25mg of Amitriptyline is used, it follows that the weight of Amitriptyline Hydrochloride should be:

 $25 \text{ mg} \times 1.132 = 28.3 \text{ mg}.$

Hence, 28.3 mg of Amitriptyline Hydrochloride is needed to make the correct standard solution.

Standard solution of Amitriptyline



Amitriptyline Hydrochloride

Amitriptyline Acidum hydrochloricum Molecular weight Molecular weight 277.4 36.5

No need for manual calculation

AP series can automatically calculate the sampling weight using the molecular amount of the standard sample, molecular weight of unnecessary sample, and the target value in order to reach the correct concentration solution.

Just weigh the target weight value on display and the target weight of the standard sample can be obtained.



"OK" mark shown when target weight is reached.

Checking weighing conditions on the same display

Series

Save Your Operation

USB Offers Greater Expandability NEW

Equipped with an RS-232C connector, a USB device and a USB host as standard. You can now simultaneously send output to both a computer and printer or connect a USB flash drive, a barcode reader, or an external numeric keypad.

Transcription errors can be avoided and data can be recorded without a computer.





(USB host: AP-W Series only)

USB and RS-232C are standard

USB host is available for AP-W Series

USB flash drive

Connecting a USB memory device allows you to record large amounts of weighing data in CSV format. Used in combination with the interval output function, it enables recording of long-term changes over time.

Example of a record: File name Date and time Weighing value



Display capture function

Weighing display can be recorded into USB memory in BMP format. User name, date/time, and setting can be shown with display information.

The user name, time, measurement conditions, pass/fail judgments, and other information displayed on screen can be saved as is, enabling the recording of measurements and checks after measurements.



Numeric keypad

Connecting a common external numeric keypad makes it easier to enter numeric values. This is especially useful for entering the mass value of weights, setting upper/lower limit values for the comparator function, or entering the sample count during piece counting mode.



Barcode reader

A barcode reader can be connected. Simply reading a barcode makes it possible to input user ID/Password. It is possible to manage sample IDs using barcodes.





An ID and password are needed to log in to the AP series if protected access is activated. With the barcode, an operator can log in by scanning the barcode instead of inputting an ID and password.

^{*} The information saved will differ depending on the function used.

^{*} The latest information can be seen from the Shimadzu website (https://www.shimadzu.com/an/balance/)

Equipped with USB as standard.*1 Includes many diverse functions to support users.

*1 AP-W Series only

Easy-to-Read Organic EL Display

(All models)


Because the pixel elements in the organic electroluminescence display emit light, the screen can be seen clearly even in dark locations. Multi-language display capability*2 provides a more intuitive operating interface. A wider viewing angle has also improved the visibility of measurement values, which helps increase the efficiency of measuring operations.

*2 English, Chinese and Japanese





Clearly visible from the side



English example

Exceptional Visibility

The visibility remains the same even when viewed from different angles. The viewing angle is a wide expanse of ±85 degrees, both vertically and horizontally. That means the display is clearly visible even when working beside the balance. A high-resolution dot-matrix display makes it easy to read detailed text.

Periodic Inspection Support Function NEW

(AP-W/AP-X Series only)

AP series supports periodic inspections. The function allows inspection of repeatability, corner load error, and linearity by simply following instructions displayed on the screen.

Example of printing



Printin	ig sample		
	REPEATABILI	TY	
	= 150 = 0.0010	g g	
N001 IL I0	= 150.0000 = 0.0000	g g	IL: Loaded weight
N002 IL I0	= 149.9999 =- 0.0001	g g	
N003 IL I0	= 149.9999 =- 0.0001	g g	
N004 IL I0	= 149.9999 = 0.0000	g g	
N005 IL I0	= 149.9999 = 0.0000	g g	
N006 IL I0	= 149.9999 = 0.0000	g g	
LOAD	RESULTS = 0.0001 (PASSED)	-	
ZERO	= 0.0001 (PASSED)	g	

Series

0.01 mg to 0.1 mg

Analytical Balances

And more...

Wide Variety of Functions to Support Users

Smart Settings (All models)

Response and stability settings can be changed during measurements with a single touch. Changing the settings for different applications can make it even easier to use.



The indicator is operated using the left and right arrow keys. Moving the setting toward [R] prioritizes response, which makes it easier to operate the balance. Conversely, moving it toward [S] makes it easier to stabilize weight values, which can improve readability in environments with vibration.







User-friendly arrow keys

Moving it left prioritizes response and moving it right prioritizes stability. Five setting levels are available.

Specific Gravity Measurement

(All models)

In combination with an optional specific gravity measurement kit, the balance can be used to measure specific gravity. Operations are simplified by a text-based navigation function. By using sinkers, the specific gravity of liquid can be measured as well. This allows measuring the specific gravity of metals, rubbers, plastics, and other materials easily.



First measure the empty weight



Then place it in the container filled with water, as instructed on the screen.



The specific gravity value is displayed using simple steps.




For Better Weighing Results

(AP-W/AP-X Series only)

Two internal weights provided


0.01 mg models are calibrated at 2 points with the internal weights (weight value and 1/2 value).



Includes Perfect Self Calibration (PSC) function

The analytical balance automatically detects any temperature changes that could affect sensitivity and automatically starts calibration.

The Clock-CAL function enables automatic calibration at a pre-specified time (for example, before starting work, during lunch, or after work hours).



Room temp Automatically calibrate sensitivity at times specified by the Clock-CAL function Sensitivity 5:00 p.m. 1 (1) Clock-CAL

22

The Reason the AP Holder in Combination with the Ionizer Can Eliminate the Influence of Static Electricity on the Weight Value

Why is the AP Holder needed as a countermeasure to static electricity?


If the AP Holder and the STABLO-AP ionizer are used together, static electricity can be quickly removed from the entire test chamber, including the surfaces of glass containers, which helps to decrease the weighing time and improve reliability.



Example of Removing Static Electricity from a Flask



The conical flask is directly placed on the pan.

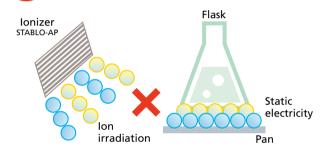


lons emitted from the ionizer cannot reach the bottom of the flask, so removal of static charge from the bottom of the flask is insufficient. Therefore, Coulomb forces act between the surrounding metal parts and the windshield door, which affects the weight value.

The bottom of the flask is in close contact with the pan, so removal of the static charge is obstructed, leading to an unstable weight value.




The conical flask is tilted using the AP Holder and placed on the pan.

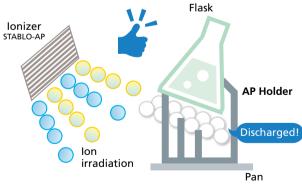

Using the AP Holder to separate the flask from the pan, the ions supplied by the ionizer reach the locations where there is static charge on the bottom of the flask. This improves the neutralization effect and results in a stable weight value.

The AP Holder can hold the container in a tilted position, so the charge can be reliably removed from the bottom of the container being mounted on the AP Holder.

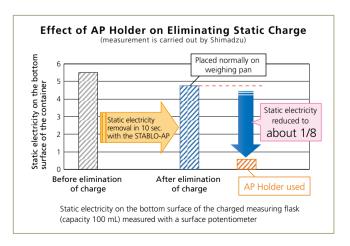

0.01 mg to 0.1 mg

AP Series

AP Series Specifications

W Series Analytical Balances

Series	W Series							
Model	AP225W	AP135W	AP125WD	AP225WD	AP124W	AP224W	AP324W	
Capacity	220 g	135 g	120 g / 52 g	220 g / 102 g	120 g	220 g	320 g	
Minimum Display	0.0	l mg	0.1 mg /	0.01 mg		0.1 mg	J	
Calibration Weight			,	Built-in*1				
External Calibration Weight Range for Span Calibration	95 to 220.00090 g (200 g)	45 to 135.00090 g (100 g)	45 to 120.00090 g (100 g)	95 to 220.00090 g (200 g)	45 to 120.009 g (100 g)	95 to 220.009 g (200 g)	95 to 320.009 g (300 g)	
Repeatability (Standard deviation)	0.015 mg (to 20 g) 0.03 mg (to 100 g) 0.05 mg (to weighing capacity)	0.03 mg (to 100 g) 0.05 mg (to 0.05 mg 0.1 mg / 0.02 mg 0.1 mg / 0.05 mg		0.1 mg / 0.05 mg	ng 0.1 mg 0		0.15 mg	
Repeatability (for Low Loads)*2	0.01 mg (5 g low loads)		0.015 mg (5 g low loads)		0.1 mg (5 g low loads)	0.1 mg (10 g low loads)	0.1 mg (20 g low loads)	
Minimum Weight*2		20	mg			200 mg		
Linearity	±0.	1 mg	±0.2 mg /±0.05 mg	±0.2 mg /±0.1 mg	±0.2	2 mg	±0.3 mg	
Response Time for Trace Measurements*3				2 sec.				
Response Time*4	8.8	sec.	2 sec. / 8 sec.			2 sec.		
USB Host (Type A)				Included	Included			
USB Device (Type B)				Included				
Recipe Compounding HPLC Buffer Solution Preparation				Included Included				
mol Conversion Function				Included				
Sample (Concentration) Preparation				Included				
Inspection Support Function				Included				
Clock-CAL				Included				
lonizer				Optional				
Operating Temperature/Humidity Range			5 ·	to 40°C 20 to 85%	* ⁵			
Sensitivity Stability Against Temperature Range			±	2 ppm/°C (10 to 30°	C)			
Pan Size	ø91 mm							
Body Dimensions	Approx. W212 × D411 × H345 mm (power supply unit included)			Approx. W212 × D367 × H345 mm				
Weight	Approx. 7.9 kg				Approx. 7.0 kg			
Display	OEL display (dot matrix)							
Input/Output Terminal		RS-2320	C (D-sub 9P plug)	USB host (Type A) l	JSB device (Type B)	Ionizer		

X Series / Y Series Analytical Balances

Series		X Series		Y Series			
Model	AP124X	AP224X	AP324X	AP124Y	AP224Y	AP324Y	
Capacity	120 g	220 g	320 g	120 g	220 g	320 g	
Minimum Display			0.1	mg	*		
Calibration Weight		Built-in			No		
External Calibration Weight Range for Span Calibration	45 to 120.009 g (100 g)	95 to 220.009 g (200 g)	95 to 320.009 g (300 g)	45 to 120.009 g (100 g)	95 to 220.009 g (200 g)	95 to 320.009 g (300 g)	
Repeatability (Standard deviation)	0.1	mg	0.15 mg	0.1	mg	0.15 mg	
Repeatability (for Low Loads)*2	0.1 mg (5 g low loads)	0.1 mg		0.1 mg (5 g low loads)	0.1 mg (10 g low loads)	0.1 mg (20 g low loads)	
Minimum Weight*2			200	mg			
Linearity	±0.2	mg	±0.3 mg	±0.2	2 mg	±0.3 mg	
Response Time for Trace Measurements*3			2 s	ec.			
Response Time*4	2 sec.						
USB Host (Type A)			Not In	cluded			
USB Device (Type B)			Inclu	ıded			
Recipe Compounding			Not In	cluded			
HPLC Buffer Solution Preparation			Not In	cluded			
mol Conversion Function		Included		Not Included			
Sample (Concentration) Preparation			Not In	cluded			
Inspection Support Function		Included		Not Included			
Clock-CAL		Included		Not Included			
lonizer		Optional		Not Included			
Operating Temperature/Humidity Range			5 to 40°C	20 to 85%* ⁵			
Sensitivity Stability Against Temperature Range	e						
Pan Size			ø91	mm			
Body Dimensions	Approx. W212 × D367 × H345 mm						
Weight	Approx. 7.0 kg Approx. 6.5 kg						
Display	OEL display (dot matrix)						
Input/Output Terminal	RS-232C (D-sub	9P plug) USB device	(Type B) Ionizer	RS-232C (D)-sub 9P plug) USB de	vice (Type B)	

^{*1} Minimum display 0.01 mg models include two internal weights (see page 22 for details).

^{*2} Be compliant with USP Chapter 41. This is the tested value by the weight of the balance's capacity 5% (or 5 grams' weight). In the case of the AP225W, the results are for tests carried out with the optional internal windbreak plate applied. The minimum weight value is affected by the installation environment, so it is necessary to measure it in the actual environment of use.

 $^{{\}bf ^{*3}}$ The response time for displaying 90% of the added sample amount value in trace measurements (from 1 mg)

^{*4} The response time value is typical.

^{*5} Non-condensing.

AP Series

AP225W AP225WD AP135W AP125WD



0.1 mg model

AP124W AP124X AP124Y AP224W AP224X AP224Y AP324W AP324X AP324Y





STABLO-AP Ionizer



EP-100 Electronic Printer



EP-110 Electronic Printer (Multifunction printer with liquid crystal display)



SMK-601 Specific Gravity Measurement Kit



Internal Windbreak Plate



AP Holder

Optional Accessories

	Static Electricity Remover STABLO-AP Ionizer
	Electronic Printer EP-100
	Electronic Printer EP-110
	Label Roll Paper for EP-100/110 (10 Rolls)
	Specific Gravity Measurement Kit SMK-601
Ï	Display Protective Cover (Set of 5)

USB Cable
RS-232C Cable
AC Adapter (Standard accessory)
Internal Windbreak Plate
RS-I/O Interface Cable
AP Holder (Standard accessory for AP225W)

Static Remover (Ionizer)



Shimadzu's proprietary ionizer for analysts troubled by static charging of samples or containers

One-touch attachment and removal adds even more convenience

— an excellent solution against **Static electricity**.

STABLO-AP provides reliable measurement by removing static electricity.



Features of STABLOAP

Static Electricity Removal by Ion Irradiation

With the high-frequency AC corona discharge method, Shimadzu's STABLO-AP ionizer provides a stable ion balance and excellent static removal performance on samples and containers.

Precision weighing work becomes remarkably efficient. Electrodes are safely housed inside the unit.


Concept of static removal



Example: negatively charged sample

AC corona discharge

Well-balanced mixture of positive/negative ions are emitted in rapid alternation.





Negative static charge is neutralized by positive ions.




AC Method Produces Excellent Ion Balance

AC method: AC voltage is applied on the discharge needle and a well-balanced mixture of positive/negative ions is emitted in rapid alternation from one electrode.

DC method: DC voltage is applied to a couple of electrodes. One is positive and the other is negative. Each electrode emits ions of one polarity only. An effective static removal angle is limited if the two electrodes are distanced. As electrodes deteriorate, initial ion balance is lost.

AC method STABLO



: Effective area

What is "ion balance"?

Ion balance is the balance of positive and negative ions that are supplied by an ionizer. If ion balance is poor, static electricity is not removed or inverse charging may result.





Not neutralized (negative charge remains)



Inversely charged (results in positive charge)

Application

Static electricity keeps the sample out of the ampoule



The sample is hard to handle because it adheres to the ampoule inlet and sides.



STABLO-AP removes the charge from the ampoule



The static charge is gone in seconds. This improves productivity.

Plastic wrap sticks to rubber gloves



Plastic wrap adheres to rubber gloves, making it difficult to work with.



Fasten STABLO-AP to the stand, and remove the static from the gloves.



The static is removed in about 10 seconds, and the plastic wrap no longer sticks.

STABLO-AP is convenient when using an electronic balance



When the powder in the Petri dish is electrically charged, and the numerical value fluctuates



When the powdered medicine paper is electrically charged, and the numerical value is unstable



When the measurement spoon is electrically charged, and bringing it near the pan affects the numerical value

Specifications

Petitieations			
Ion Generation Method	AC corona discharge method		
lon Balance	±10 V		
Effective Static Removal Range	Approx. 400 mm from the outlet		
Static Elimination Time (approx.)	1 second (Typical value) (from ±1000 V to ±100 V)		
Ozone Concentration	0.06 ppm		
Electrode Probes	Tungsten (durability: 30,000 hours)		
Weight	Approx. 710 g (Main unit: 395 g, Stand: 315 g)		
Operating Temperature and Humidity	0 °C to + 40 °C, 25 % RH to 85 % RH (non-condensing)		
Rated Electric Power Supply	DC 24 V, 1.0 A		

Analytical Balances



Multi Functional Analytical Balances

UniBloc Analytical Balances

AUW-D series dual-range semi-micro balances AUW/AUX/AUY series analytical balances

Excellent Weighing Performance

 Compact UniBloc mechanism and digital processing technology produce fast response and stability at the same time.

For Applications

- Shimadzu's unique Balance Keys (https://www.shimadzu.com/an/balance/balance_keys/)
- Measurement results can be transmitted to Excel® or other Windows® applications without installing any additional software on your computer. All you have to add is one RS-232C cable.
- Piece counting, various mass units, below-weigh hook, specific gravity measurement software are all standard features.





AUW Series






Choose the model according to your field

Excellent response, stability and zero return performance - in a semi-micro balance.



PSC (Perfect Self-Calibration) (AUW-D/AUW/AUX series only)


Automatically calibrates the balance if an ambient temperature change occurs that could affect sensitivity.





Clock-CAL

This automatically calibrates the balance at pre-specified times (such as before starting work, during lunch, or after work hours).





Internal Calibration (AUW-D/AUW/AUX series only)

The balance has built-in motor-driven calibration weights. Sensitivity can be calibrated whenever needed with a single key press.



ISO Calibration Report

Simply connect an optional printer to automatically print out which balance was calibrated when, and the calibration results. Absolutely no troublesome settings are required. Furthermore, the current date and time can be printed at anytime during measurement.



Interval Timer (AUW-D/AUW/AUX series only)

Data can be automatically output at time intervals set in the range from 1 second to 99 minutes 59 seconds. This function can be combined with Balance



Piece Counting

A built-in piece counting function enables balances to be used as parts counters (piece scales).



RS-232C Interface

All models are equipped with an RS-232C interface for easy integration with other devices and computers.



Specific Gravity Measurement

Installing the optional SMK-401 specific gravity measurement kit transforms the balance into a dedicated instrument for measuring specific gravity or density. Specific gravity measurement software is already installed in the Shimadzu balance.



Measuring Carats

The balance supports measurements in carats. momme, percent, and a variety of other measurement units. (The unit momme is only used for measuring pearls.)

AUW-D Series	Uni Bloc	PSC COA CAL MATERIAL BUILT-IN ISO	Balance RS-ZZCC PCS CAPAT Dailor State Sta
AUW Series	Uni Bloc	PSC COL CAL BUILTING ISO	Balance RS-220C PCS CAPAR Analysis States 5 10 12 12 12 12 12 12 12 12 12 12 12 12 12
AUX Series	Uni Bloc	PSC Built-in ISO	Balance RS-220C PCS CAPAR Language State 5 To Capara Language State 5 To Ca
AUY Series	Uni Bloc		Balance RS-2202 PCS CARAIT Making Company Comp

AU Series

	AUW-D Series		AUW Series				AUX Series	AUY Series			
Model name	AUW220D	AUW120D	AUW320	AUW220	AUW120	AUX320	AUX220	AUX120	AUY220	AUY120	
Capacity	220 g/82 g	120 g/42 g	320 g	220 g	120 g	320 g	220 g	120 g	220 g	120 g	
Minimum Display	0.1 mg/0.01 mg		0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	
Pan Size (mm)		Approx. 80 dia.									
Body Dimensions		Approx. W217 × D356 × H338 mm									
Weight		Approx. 7 kg									

Optional Accessories

Description
Static Electricity Remover STABLO-AP Ionizer
Electronic Printer EP-100
Electronic Printer EP-110
Specific Gravity Measurement Kit SMK-401
In-use Protective Cover
RS-232C Cable
USB Conversion Cable
Application Keyboard AKB-301
Foot Switch FSB-102PK
Foot Switch FSB-102TK



Electronic Printer EP-100



Electronic Printer EP-110



Application Keyboard AKB-301



STABLO-AP



Specific Gravity Measurement Kit SMK-401

AT-R Series

Analytical Balances

AT-R series

Basic Model with Improved Convenience

- Freely set responsiveness or stability
- Perform stable measurements in combination with an ionizer
- Connect with a computer via USB or RS-232C



Basic Models of Analytical Balances








PSC (Perfect Self-Calibration) (ATX-R only)

Automatically calibrates the balance if an ambient temperature change occurs that could affect sensitivity.





Internal Calibration (ATX-R only)

The balance has built-in motor-driven calibration weights. Sensitivity can be calibrated whenever needed by a single key press.



Computer Connection Function

Systems can be connected to a computer via an optional cable/adapter kit. For more details, visit the Shimadzu website.



RS-232C Interface

All models are equipped with an RS-232C interface for easy integration with other devices and computers.



USB Interface

A USB connector is built in for connecting to a PC.



Piece Counting

A built-in piece counting function enables balances to be used as parts counters (piece scales).



Checkweighing

This displays pass, high, or low judgments.



Measuring Carats

The balance supports measurements in carats, momme, percent, and a variety of other measurement units. (The unit momme is only used for measuring pearls.)



Percentage Measurement

Measures a percentage value with respect to a preset reference.



Formulation Mode

This is convenient when formulating (preparing) multiple substances.



Easy Setting







Stability-focused (S) when vibrations become a concern



ATX-R Series	Unit
--------------	------



































AT-R Series

ATY-R Series

Model	ATX324R	ATX224R	ATX124R	ATX84R	ATY324R	ATY224R	ATY124R	ATY64R		
Capacity	320 g	220 g	120 g	82 g	320 g	220 g	120 g	62 g		
Minimum Display		0.1 mg								
Pan Size (mm)		Approx. 91 dia.								
Dimensions		Approx. W213 × D356 × H338 mm								
Weight		Approx	. 6.2 kg		Approx. 6.0 kg					

Optional Accessories

Description					
Static Electricity Remover STABLO-AP Ionizer					
Electronic Printer EP-100					
Electronic Printer EP-110					
USB Cable Set					
SMK-501 Specific Gravity Measurement Kit					
AP Holder					
Protective Cover (5 pc set)					
AC Adapter (Provided with the main unit)					









Electronic Printer EP-100

Electronic Printer EP-110



Specific Gravity Measurement Kit SMK-501



AP Holder

0.1 mg

Analytical Balances

Analytical Balances

ATseries

Economical Analytical Balance Equipped with UniBloc

- Adopts UniBloc, which provides excellent impact resistance, responsiveness, and stability
- Equipped with the Easy Setting function, so responsiveness and stability can be adjusted during measurements
- Buy a separately available I/O-RS cable to import the results to a PC (Equipped with the Balance Keys function)

Basic Models of Analytical Balances







Internal Calibration (ATX only)

The balance has built-in motor-driven calibration weights. Sensitivity can be calibrated whenever needed by a single key press.



Piece Counting

A built-in piece counting function enables balances to be used as parts counters (piece scales).



Checkweighing

This displays pass, high, or low judgments.



Formulation Mode

This is convenient when formulating (preparing) multiple substances.



Percentage Measurement

Measures a percentage value with respect to a preset reference.



Measuring Carats

The balance supports measurements in carats, momme, percent, and a variety of other measurement units. (The unit momme is only used for measuring pearls.)



Easy Setting







Response-focused (R) for weighing process



Stability-focused (S) when vibrations become a concern



Uni Bloc











ATX Series











ATX/ATY Series

Model	ATX324	ATX224	ATX124	ATX84	ATY324	ATY224	ATY124	ATY64		
Capacity	320 g	220 g	120 g	82 g	320 g	220 g	120 g	62 g		
Minimum Display	0.1 mg									
Pan Size (mm)		Approx. 91 dia.								
Dimensions		Approx. W213 × D356 × H338 mm								
Weight		Approx	. 6.2 kg		Approx. 6.0 kg					

Optional Accessories

Description
Description
Static Electricity Remover STABLO-AP Ionizer
Electronic Printer EP-100
Electronic Printer EP-110
I/O-RS Conversion Cable
USB–Serial Adapter
Protective Cover (5 pcs)
AC Adapter (Provided with main unit)



STABLO-AP



Electronic Printer EP-100



Electronic Printer EP-110



I/O-RS Conversion Cable



USB-Serial Adapter

Series

0.001 g to 0.1 g

Electronic Balances

Multi Functional Top-Loading Balances

Top-loading Balances with the Fastest Response Performance in Its Class



Large Pan with 0.01 g Minimum Display Value

UP2202X UP2202Y UP4202X UP4202Y UP6202X UP6202Y



Large Pan with 0.1 g Minimum Display Value

UP4201X UP4201Y UP8201X UP8201Y



Small Pan with 0.001 g Minimum Display Value

UP223X UP223Y UP423X UP423Y UP623X UP623Y UP823X UP823Y UP1023X UP1023Y



Small Pan with 0.01 g Minimum Display Value

UP422X UP422Y UP822X UP822Y





PSC (Perfect Self-Calibration) (UP-X series only)

Automatically calibrates the balance if an ambient temperature change occurs that could affect sensitivity.



Clock-CAL (UP-X series only)

This automatically calibrates the balance at pre-specified times (such as before starting work, during lunch, or after work hours).



Internal Calibration (UP-X series only)

Enables calibration by pressing a single key with one finger. That ensures calibration can be performed



Printout with Date and Time

If a printer (optional) is connected, then data can be marked with the date and time. Calibration results can also be marked with date and time, which is perfect for managing measurements or establishing traceability as required by GLP/GMP/ISO 9001 standards.



ISO Calibration Report

Simply connect an optional printer to automatically print out which balance was calibrated when, and the calibration results. Absolutely no troublesome settings are required. Furthermore, the current date and time can be printed at anytime during measurement.



Backlight LCD

This backlit LCD can be clearly read even in the darkest of environments.



Checkweighing

By specifying upper and lower limit values in advance, the comparator indicates whether the sample weight passes the criteria, is too heavy, or is



Comparator Output

Acceptable, high, or low weight results or other pass/fail results can be indicated by an audible sound or output externally as a contact signal. (Optional comparator audible indicator or relay output interface required.)



Measuring Carats

The balance supports measurements in carats. momme, percent, and a variety of other measurement units.

(The unit momme is only used for measuring pearls.)



Computer Connection Function

Systems can be connected to a computer via an RS-232C cable or using a USB-serial adapter kit. For more details visit the Shimadzu website



Piece Counting

A built-in piece counting function enables the balance to be used as a parts counter (counting balance).



Specific Gravity Measurement Function

The built-in specific gravity measurement function is based on the liquid immersion method. By installing the specific gravity measurement kit (optional), the balance can be used as a hydrometer.





UP-X Series


Model name	UP223X	UP423X	UP623X	UP823X	UP1023X	UP2202X	UP4202X	UP6202X	UP422X	UP822X	UP4201X	UP8201X
Capacity	220 g	420 g	620 g	820 g	1020 g	2200 g	4200 g	6200 g	420 g	820 g	4200 g	8200 g
Minimum Display	0.001 g	0.001 g	0.001 g	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g
Pan Size (mm)	Approx. 108 × 105					Approx. 170 × 180			Approx.	108 × 105	Approx. 170 × 180	

UP-Y Series

Model name	UP223Y	UP423Y	UP623Y	UP823Y	UP1023Y	UP2202Y	UP4202Y	UP6202Y	UP422Y	UP822Y	UP4201Y	UP8201Y
Capacity	220 g	420 g	620 g	820 g	1020 g	2200 g	4200 g	6200 g	420 g	820 g	4200 g	8200 g
Minimum Display	0.001 g	0.001 g	0.001 g	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g
Pan Size (mm)	Approx. 108 × 105					Approx. 170 × 180			Approx.	108 × 105	Approx. 170 × 180	

Response for Weighing Minute Quantities

Large-pan model with 0.01 g minimum display value Small-pan model with 0.001 g minimum display value

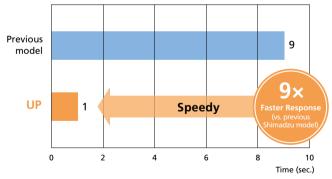

Measurement Conditions:

Large-pan model with 0.01 g minimum display value and 0.1 g load Small-pan model with 0.001 g minimum display value and 0.01 g load

Optional Accessories

	Description
Static Elec	tricity Remover STABLO-AP Ionizer
Electronic	Printer EP-100
Electronic	Printer EP-110
RS-232C C	able 25P–9P (1.5 m)
USB–Seria	Replacement Kit
Applicatio	n Keyboard AKB-301
Windbrea	k Set *1
Windbrea	k Set (For large pan) *2
Glass Wind	dbreak WBC-102
Large Size	Windbreak WBC-502
In-use Prot	tective Cover (3 pcs) (For large-pan models with 0.01 g min. display value)
In-use Prot	tective Cover (5 pcs) (For large-pan models with 0.1 g min. display value)
In-use Prot	tective Cover (5 pcs) (For small-pan model)
In-use Prot	tective Cover (5 pcs) (For display and key part)
Animal Bu	cket Set (For large-pan models with 0.01 g minimum display value)
Animal Bu	cket Set (For large-pan models with 0.1 g minimum display value)
	avity Measurement Kit SMK-101A (For large-pan model) proximately 2 kg for weighing capacity)
Specific G	ravity Measurement Kit SMK-102 (For small-pan model)
Remote D	isplay RDB-201
Remote D	isplay RDB-202
Relay Out	put Interface IFB-RY1
RY1 Conne	ection Cable
AC Adapte	er *3

- *1 Included standard with small pan models with 0.001 g minimum display value.
- *2 Included standard with large pan models with 0.01 g minimum display value. *3 Included standard with main unit.

Electronic Balances

Electronic Balances

UW/UX series

Multi Functional Top-Loading Balances

Top-loading Balances with UniBloc Technology







UW420S UX420S UW820S UX820S



UW220H	UX220H
UW420H	UX420H
UW620H	UX620H
UW820H	UX820H
UW1020H	UX1020I

* Windbreak can be removed.

UW8200S


UW2200H

UW4200H UW6200H



PSC (Perfect Self-Calibration) (UW only)


Automatically calibrates the balance if an ambient temperature change occurs that could affect sensitivity.





Clock-CAL (UW only)

This automatically calibrates the balance at pre-specified times (such as before starting work, during lunch, or after work hours).





Internal Calibration (UW only)

Press just two keys to calibrate the balance whenever calibration is necessary.



ISO Calibration Report

Simply connect an optional printer to automatically print out which balance was calibrated when, and the calibration results. Absolutely no troublesome settings are required. Furthermore, the current date and time can be printed anytime during measurement







Backlight LCD

The backlight LCD display can be clearly read in the darkest of environments.



Checkweighing

When upper and lower thresholds are set, the balance indicates if the sample weight is within the range (GO), over (HI) or under (LO).



Piece Counting

A built-in piece counting function enables the balance to be used as a parts counter (counting balance).



Specific Gravity Measurement Function

The built-in specific gravity measurement function is based on the liquid immersion method. By installing the specific gravity measurement kit (optional), the balance can be used as a hydrometer.



Computer Connection Function

Systems can be connected to a computer via an RS-232C cable or using a USB-serial adapter kit. For more details, visit the Shimadzu website.



Data transfer port of UW/UX Series



Measuring Carats

The balance supports measurements in carats, momme, percent, and a variety of other measurement units. (The unit momme is only used for measuring pearls.)





















Model name	UW220H	UW420H	UW620H	UW820H	UW1020H	UW420S	UW820S	UW2200H	UW4200H	UW6200H	UW4200S	UW8200S
Capacity	220 g	420 g	620 g	820 g	1020 g	420 g	820 g	2200 g	4200 g	6200 g	4200 g	8200 g
Minimum Display	0.001 g	0.001 g	0.001 g	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g
Pan Size (mm)		Approx. 108 × 105							App	rox. 170 ×	180	

UX Series

Model name	UX220H	UX420H	UX620H	UX820H	UX1020H	UX420S	UX820S	UX2200H	UX4200H	UX6200H	UX4200S	UX8200S
Capacity	220 g	420 g	620 g	820 g	1020 g	420 g	820 g	2200 g	4200 g	6200 g	4200 g	8200 g
Minimum Display	0.001 g	0.001 g	0.001 g	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g
Pan Size (mm)		Approx. 108 × 105							App	rox. 170 ×	180	

Description
Static Electricity Remover STABLO-AP Ionizer
Electronic Printer EP-100
Electronic Printer EP-110
RS-232C Interface IFB-102A (Needed only for multiple connection)
Small Size Windbreak (For models with capacity of 300 g to 620 g only) (Std. acc. for models with readability of 0.001 g)
Glass Windbreak (For models with capacity of 220 g to 820 g only)
Large Size Windbreak (For all models)
Specific Gravity Measurement Kit SMK-101 (For large pan 170 × 180 mm)
Specific Gravity Measurement Kit SMK-102 (For small pan 108 × 105 mm)
Protective In-use Cover for Key Panel and Display (5 pcs)
Small Animal Bucket Set (For large-pan models only)
Angle Adjuster and Wall Hook for Remote Display
Stand for Remote Display (1 m high)
Foot Switch FSB-102PK (For printing)
Foot Switch FSB-102PK (For taring)
RS-232C Cable, for IBM PC/AT Compatibles (25P–9P, Null modem, 1.5 m)
RS-232C Cable, for Multiple Connections (25P–25P, Null modem, 1.5 m)
Application Keyboard AKB-301
Remote Display Unit RDB-201 with Operation Keys
Remote Display Unit RDB-202



Glass windbreak WBC-102



Large size windbreak WBC-502



STABLO-AP



Application Keyboard AKB-301

Electronic Balances

Electronic Balances

TW/TX/TXB series

The beginning of the new standard. Extremely capable, but easy to operate.









Internal Calibration

Press just two keys to calibrate the balance whenever calibration is necessary (TW only). Calibration is very fast, taking only 15 sec.



Easy Setting


Quickly adjust the desired ratio of stability and response for every application, even during measurement, with one-touch operation.





Menu Operation Key

Menu navigation keys are separated from weighing operation keys and arranged in a familiar 5-way navigation circle. Up, Down, Right, Left and Enter are the simple operational steps.





Dry Battery Operation

Power the TXB series balances with an AC adapter or



Piece Counting

Unit weights of up to five different samples can be easily entered, stored and recalled for use.



Measuring Carats

In addition to grams (g), weigh in %, number of pieces, ct, kg, mg, lb, oz, TTI, etc. or a custom conversion unit, more than 20 units in all. Change quickly from display of % or counting to gram weight (g) display.



Checkweighing


Compare samples to target values or pass/fail criteria and clearly indicate the results.

TW Series Uni Bloc



















TXB Series



TW223L TW323L TW423L TX223L TX323L TX423L



TW Series

Model name	TW223L	TW323L	TW423L	TWC323L	TWC623L			
Capacity	220 g	320 g	420 g	320 ct (64 g)	620 ct (124 g)			
Minimum Display	0.001 g	0.001 g	0.001 ct (0.0002 g)					
Pan Size (mm)		Approx. ø110		Approx. ø80				
Dimensions		Approx. W206 × D291 × H241 mm						
Weight	F	Approx	. 4.1 kg					

TX2202L TX3202L TX4202L



TWC323L TXC323L TWC623L TXC623L

TX Series

Model name	TX223L	TX323L	TX423L	TX2202L	TX3202L	TX4202L	TXC323L	TXC623L
Capacity	220 g	320 g	420 g	2200 g	3200 g	4200 g	320 ct (64 g)	620 ct (124 g)
Minimum Display	0.001 g	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.001 ct (0.0002 g)
Pan Size (mm)		Approx. ø110			rox. W167 × 🛭	Approx. ø80		
Dimensions	Approx. W	/206 × D291 ×	H241 mm	Approx. V	V200 × D291 >	Approx. W206 × D291 × H241 mm		
Weight	,	Approx. 3.8 kg]	,	Approx. 2.8 kg	3	Approx	. 3.8 kg



TXB2201L TXB6201L TXB4201L TXB6200L



TXB222L TXB622L TXB422L TXB621L

TXB Series

Model name	TXB422L	TXB622L	TXB4201L	TXB6201L					
Capacity	420 g	620 g	4200 g	6200 g					
Minimum Display	0.01 g	0.01 g	0.1 g	0.1 g					
Pan Size (mm)	ø1	10	ø160						
Dimensions	Ар	Approx. W199 × D260 × H77 mm							
Weight		Approx. 1.5 kg							

	Description	
Electro	ic Printer EP-100	
Electro	ic Printer EP-110	
RS-232	Cable	
In-use	rotective Cover	
In-use	rotective Cover for Display	
USB Co	version Kit	



Electronic Printer EP-100



Electronic Printer EP-110

Top-Loading Balances



Basic Top-Loading Balances



BL_{Series}







BL Series

Model name	BL-220H	BL-320H	BL-320S	BL-620S	BL-2200H	BL-3200H	BL-3200S
Capacity	220 g	320 g	320 g	620 g	2200 g	3200 g	3200 g
Minimum Display	0.001 g	0.001 g	0.01 g	0.01 g	0.01 g	0.01 g	0.1 g
Pan Size (mm)		W100 × D100			W160	× D124	•



Data transfer port of BL Series

Description
Electronic Printer EP-100
Electronic Printer EP-110
In-use Protective Cover



Electronic Printer EP-100

Electronic Printer EP-110

Basic Portable Electronic Balances

Portable Electronic Balances



Precision without Compromise



ELB series






ELB Series

Model name	ELB120	ELB200	ELB300	ELB600	ELB600S	ELB1200	ELB2000	ELB3000	ELB6000S	ELB12K
Capacity	120 g	200 g	300 g	600 g	600 g	1200 g	2000 g	3000 g	6000 g	12 kg
Minimum Display	0.01 g	0.01 g	0.01 g	0.05 g	0.1 g	0.1 g	0.1 g	0.1 g	1 g	1 g
Pan Size (mm)		ø110				\	N170 × D130)		



Data transfer port of ELB Series





Electronic Printer EP-100



BW-K/BX-K Series

Precision Platform Balances

Precision Balances for Heavy Samples

BW-K/BX-K series

The Shimadzu precision platform balances have been engineered with the innovative UniBloc mechanism since 1989. Powerful features support any imaginable weighing application. The BW-K Series includes internal calibration weight.



BW12KH





Hook assy for below weighing (Optional)

Data transfer port of BW-K/BX-K Series



BW-K Series

















BX-K Series



















BW-K/BX-K Series

Model name	BW12KH	BW22KH	BW32KH	BW32KS	BW52KS	BX12KH	BX22KH	BX32KH	BX32KS	BX52KS
Capacity	12 kg	22 kg	32 kg	32 kg	52 kg	12 kg	22 kg	32 kg	32 kg	52 kg
Minimum Display	0.1 g	0.1 g	0.1 g	1 g	1 g	0.1 g	0.1 g	0.1 g	1 g	1 g
Pan Size (mm)		W345 × D250								

	Description
RS-2320	Interface IFB-102A (For multiple connections)
Electro	nic Printer EP-100
Electro	nic Printer EP-110
Foot Sv	vitch FSB-102PK (For printing)
Applica	tion Keyboard AKB-301
USB-Se	rial Conversion Kit
RS-2320	C Cable
Below-	weigh Hook



Electronic Printer EP-100



Electronic Printer EP-110



Application Keyboard AKB-301

Moisture Analyzer

MOC-120H

Moisture Analyzer with a Wide Sample Pan

Measure the Moisture Ratio of Even Large or Large Amounts of Samples

- The moisture ratio is found by heating the sample with the built-in infrared heater.
- The sample pan measures 130 mm in diameter, which is optimal for large and large amounts of samples.
- Importing results to a PC is easy (equipped with the Balance Keys function).
- Equipped with the UniBloc aluminum block mass sensor.

MOC-120H







MOC-120H

Model	MOC-120H
Measurement Method	Infrared heating/dry mass measurement
Pan Size	130 mm dia
Minimum Weight Displayed	0.001 g
Moisture Ratio Measurement Range	0.01 to 100.00 %
Minimum Moisture Ratio Displayed	0.01 %
Maximum Sample Quantity	120 g
Measurement Modes	Automatic operation mode, Timed operation mode, High-speed drying mode, Low-speed drying mode
Drying Heat Source	Medium wave infrared quartz heater
Temperature Settings Range	30 to 200 °C (1 °C steps)
Unit Dimensions and Weight	W 220 × D 415 × H 190 mm, 4.5 kg
Operational Temperature and Humidity Range	5 to 40 °C, relative humidity of 85 % max.
Required Power Supply	100 to 120/220 to 240 VAC, 640 W max.
Accessories	Sample pan × 2, pan holder, windbreak, sample pan tongs, aluminum sheet × 20, spatula

Printer



Drying conditions during measurement and the final measurement value can be graphed and printed.

Optional Accessories

Description	
Printer Set Includes a Connection Cord and 1 Roll of Printer Paper (Therm	al paper)
Printer Paper (10 rolls)	
RS-232C Cable	
Sample Pan	
Aluminum Sheets (500 pcs)	
Temperature Calibration Kit *1	
Protective Display Cover (5 pcs)	

*1 Temperature calibration using the optional Temperature Calibration Kit may be necessary depending on the measurement sample and the measurement conditions. Temperature calibration makes it possible to control the drying temperature of the measurement sample more accurately.

Warning

- Use this balance to heat samples to evaporate moisture for measurement.
- The built-in heater will be hotter than the set temperature.
 Samples must not be measured if there is a risk of an explosion or fire, or
- a dangerous chemical reaction from heating.

Sample Output from Optional Printer

[Graph Format (GRP)]			

Maker : SHIMADZU CORP		Company name	: Shimadzu Corporation
Model: MOC-120H		– Model	: MOC-120H
S/N : D207300000		– Serial no.	: D207300000
ID : ABCD-123		- Instrument ID	: ABCD-123
Sample Code : B-20		- Sample code	: B-20
Date/Time : 2007.08.08/15:07		Measurement date/time	: 15:07 Aug. 8, 2007
Condition No : 0		 Measurement conditions storage area 	:0
Unit : Dry Base Moist.		Measurement reference	: Dry basis moisture ratio
Mode : Compare		Measurement mode	: Comparative measurement
Setting Temp. : 1100		Drying temperature	: 110 °C
Auto Stop Cond. : 0.05%		Automatic ending conditions	: 0.05 %
Pred. Tol. : 0.5		Predictive convergence range	: 0.5
Wet-Mass : 5.6892	•	 Un-dried mass 	: 5.6892 g
Time Temp. Moist.			
(min) (C) (X) 0 4 8 12	16 20%		
0.0 35 0.00 ▶			
0.5 60 0.581* 1 1 1 1 1 1	111		
1.0 106 5.45			
1.5 110 7.64 *	1 1 1		
2.0 110 9.09			
2.5 110 10.31	!!!		
3.0 110 11.05			
3.5 110 11.731	!!!		
4.0 110 12.17		Measurement time	
5.0 110 12.681			
5.5 110 13.21		Drying temperature	
6.0 110 13.41		Measurement value (%)	
6.5 110 13.64			
7.0 110 13.77			
7.5 110 13.901			
Predicted: 14.59	للسننان	Predicted measurement value	
8.0 110 14.06		Fredicted measurement value	
8.5 110 14.14			
9.0 110 14.22			
	iii l		
10.0 110 14.43			
	iii II		
	/		
Dry-Mass : 4.8637 €		— Dried mass : 4.8637 q	
Dry-Mass : 4.8637		Dried mass . 4.8637 g	
***************************************	***********		

0.001 g / 0.01 %

Moisture Analyzer

MOC63u

Easy, Reliable Moisture Content Measurements

This Unit Makes Moisture Content Measurements Quick and Easy

- The moisture ratio is found by heating the sample with the built-in halogen heater to drive out the moisture
- The measurement procedure is simple. Just close the heater cover to start the measurement (automatic starting mode).
- Measurements are faster than the loss on drying method using a dryer.
- A USB connector makes connecting to a PC easy (built-in Balance Keys
- Equipped with the UniBloc aluminum block mass sensor.



This product is certified as Shimadzu's Eco-Products Plus. Energy Saving: Power consumption reduced by 30% as compared to a conventional Shimadzu product.



The sample pan size is a spacious 95 mm dia.

Generally, the wider, thinner, and more uniformly the sample is spread, the more precise the measurement. Uniform heating is provided by adopting a cleverly shaped





- 1 A cross-shaped key layout has been adopted for excellent operability.
- (2) A real-time indicator has been adopted, which blinks to show the measurement status.
- (3) The results are shown as a percentage using a backlit LCD to enhance visibility.
- (4) Graphics are provided to let you confirm the pan status in real time.

The sample is easy to see! Wide observation window

A Total of Five Modes Makes This Balance Compatible with a Variety of Sample Measurements


Ending Modes

Automatic Ending Mode

This automatically ends measurement when the moisture change (% margin) over 30 seconds drops below a set value.

Timed Ending Mode

This automatically ends measurement after a preset amount of time (t1).



Alternate Drying Modes


The sample is dried at the highest temperature for the initial drying stage, and when the moisture has been reduced, it returns to the set temperature, shortening the measurement time.

Slow Drying Mode

This gently heats samples that might form a surface film or are prone to degrading at high temperatures.

Step Drying Mode

Drying conditions are changed step by step for samples that contain a lot of moisture, such as surface water or crystallization





MOC63u











MOC63u

	Model	MOC63u				
Capacity	Max. Sample Quantity	60 g				
Сараспу	Min. Sample Quantity	0.02 g				
Minimum	Mass	0.001 g				
Display	Moisture Ratio	0.01 %				
Repeatability *	1	0.15 % (2 g), 0.05 % (5 g), 0.02 % (10 g)				
Heat Source	Method	Halogen (straight tube)				
neat source	Power	Rated at 400 W				
Temperature Se	ettings	50 to 200 °C (1 °C interval) (up to 1 hour for settings over 180 °C)				
Display		Backlit LCD				
Pan Size		95 mm dia.				
Dimensions (m	m)	Approx. W 202 × D 336 × H 157				
Weight		Approx. 4.2 kg				
Rated Power		430 VA				
Ambient Temp	erature	5 to 40 °C, relative humidity of 85 % max.				
		Standard drying mode (Automatic ending/timed ending)				
Measurement I	Madas	Rapid drying mode (Automatic ending/timed ending)				
Measurement	vioues	Slow drying mode (Automatic ending/timed ending)				
		Step (3-stage) drying mode (Automatic ending/timed ending)				
Time Settings		1 to 240 min, or continuous (up to 12 hours)				
		USB				
External Outpu	t	Data I/O printer (EP-100/EP-110) output				
		RS-232C (D-sub 9P)				
Storage of Mea	surement Conditions	10 sets				
Data Memory		100 items				
		Sample pans (3 aluminum pans), pan holder, windbreak,				
Standard Acces	sories	board, aluminum sheets (50), pan handler, power cable,				
		spare fuses (2), protective display cover, hexagonal wrench				

^{*1} The repeatability (standard deviation) value is from a standard measurement (sample: sodium tartrate dihydrate). This value is not guaranteed for all samples, environments, and measurement conditions

Optional Accessories

Description	
Electronic Printer EP-100	
Electronic Printer EP-110	
Protective Display Cover (5 pcs)	
Aluminum Pans (Disposable) (50 pcs)	
Fiberglass Sheets (For liquid sample measurements) (100 pcs)	
Temperature Calibration Kit	
Sample Pan (Stainless steel) (5 pcs)	
Sample Pan (Aluminum) (5 pcs)	
RS-232C Cable	
USB Cable Set	
Sample Pan Handler (Stainless steel)	
Halogen Heater (For replacement) *2	
Power Cable	

*2 The halogen heater can be removed and replaced by the user. Note: For delivery related matters, contact your Shimadzu representative.



Warning

- Use this balance to heat samples to evaporate moisture for measurement.
- The built-in heater will be hotter than the set temperature.
 Samples must not be measured if there is a risk of an explosion
- or fire, or a dangerous chemical reaction from heating.

Simple Operation

Select the automatic starting mode, place the sample, and close the heater cover to start the measurements. The preparation for measurement is so simple that you do not even have to press the start key.




A Wealth of PC Connection Functions

A built-in USB connector allows connecting to a PC. It can be used in conjunction with the Balance Keys function.


For USB port connections, check the Shimadzu website or contact your Shimadzu representative.





Sample Printout

• Sample Measurement Results Output

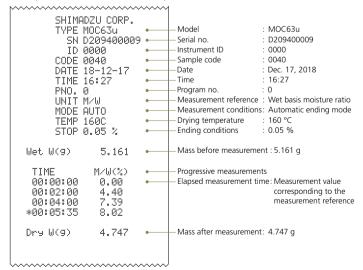

Using the EP-100/EP-110

MOC63u 0.001 g / 0.01 %

Moisture Analyzer

Moisture Analyzer

MOC63u Application Examples



Food Industry


Measurement of Milk

- Fiberglass sheets for liquid measurement were used to promote liquid evaporation.
- Two measurement conditions were used, timed ending and automatic ending modes. Essentially the same average values were obtained. With samples whose principal component has a relatively high evaporation temperature and also contains moisture, the same results will be obtained regardless of the mode used.

Measurement Conditions: 140 °C/Timed 10 min

	MOC63u	
	Sample Mass (g)	Moisture Content (%)
1st	1.081	87.70
2nd	1.025	87.61
3rd	1.031	87.68
Average		87.66
Standard Deviation		0.047
CV (%)		0.05

Drying Curve for Milk in Timed Ending Mode



Milk before Drying



(Before measurement) 1 g of milk was dripped on to a fiberglass sheet for liquid measurement.

Milk after Drying



(After measurement) The moisture has evaporated from the milk, and the remaining fats have yellowed slightly.

Food Industry

Pharmaceuticals and **Cosmetics Industries**


Measurement of Corn Starch

- Approx. 5 g of corn starch was added to the pan and was spread over the entire surface using the tip of a spoon.
- · No change in appearance was evident after drying.
- Favorable repeatability of 1 % max. was obtained.

Measurement Conditions: 180 °C/Automatic 0.02 %

MOC63u									
	Measurement Time	Moisture Content (%)							
1st	9:49	5.133	12.27						
2nd	9:14	4.910	12.10						
3rd	9:12	5.097	12.14						
Average	***************************************	!	12.17						
Standard Deviation			0.09						
CV (%)			0.73						

Drying Curve for Corn Starch in Automatic Ending Mode



Corn Starch before Drying



(Before measurement) The sample powder was spread evenly over the pan.

Corn Starch after Drying



(After measurement) There was basically no change in appearance.

The table below summarizes moisture ratio measurements for various samples using the moisture analyzer.

	Sample	Measuren	nent Mode	Set Temperature	Measurement	Moisture		
Sample	Quantity	Ending Conditions	Finishing Conditions (% or min)	(°C)	Time (min)	Ratio (%)	CV (%)	
Dog food	1 g	AUTO	0.05 %	160	5:48	6.45	3.17	
Table salt	5 g	TIME	10 min	200	10:00	0.08	6.93	
Instant coffee	1 g	TIME	10 min	120	10:00	7.43	1.18	
Coffee beans (raw)	5 g	AUTO	0.05 %	140	17:30	9.32	1.68	
Coffee beans (roasted)	3 g	AUTO	0.05 %	140	7:06	2.68	3.73	
Green tea	5 g	AUTO	0.05 %	120	9:05	3.76	0.41	
Corn starch	5 g	AUTO	0.02 %	180	9:25	12.17	0.73	
Sugar (granulated sugar)	5 g	AUTO	0.05 %	160	1:02	0.13	0.01	
White rice	6 g	AUTO	0.05 %	200	13:55	14.48	0.42	
Mayonnaise	1 g	TIME	10 min	160	10:00	20.61	0.46	
Orange juice	1 g	AUTO	0.05 %	140	10:09	88.89	0.09	
Milk	1 g	AUTO	0.05 %	140	7:30	87.36	0.04	
Chocolate	3 g	AUTO	0.01 %	140	6:18	2.36	1.49	
Rolled oats	6 g	AUTO	0.05 %	200	10:05	12.65	0.14	
Tomato ketchup	2.5 g	AUTO	0.1 %	140	19:47	69.40	0.16	
rozen sweets	2.5 g	TIME	12 min	140	12:00	84.53	0.22	
Oried mangoes	5 g	AUTO	0.05 %	120	28:27	6.62	12.10	
Palm oil	2.5 g	TIME	5 min	120	5:00	0.41	3.70	
Hand soap	1 g	AUTO	0.05 %	200	21:36	88.89	0.39	
ipstick	1 g	TIME	3 min	100	3:00	0.73	9.37	
Plastic (PMMA pellet)	10 g	TIME	25 min	100	25:00	0.13	4.56	
Photocopier paper	1 g	AUTO	0.05 %	200	1:50	7.84	0.71	
Sodium tartrate dihydrate	5 g	TIME	15 min	160	15:00	15.80	0.04	
Detergent (powdered)	5 g	AUTO	0.05 %	160	13:08	9.79	1.59	
Solid soap	3 g	TIME	16 min	200	16:00	9.09	1.66	
Water-based paint	1 g	AUTO	0.05 %	200	9:27	52.39	0.75	
Sludge cake	2 g	AUTO	0.05 %	200	21:31	81.55	0.40	
Potting soil	5 g	AUTO	0.05 %	120	15:30	33.40	2.16	
Sawdust	4 g	AUTO	0.05 %	160	8:27	34.38	0.91	
Baked sweets	3 g	RAPID	Step 1 3.0 % Step 2 0.1 %	Step 1 200 Step 2 110	5:10	7.6	30.26	
Dengakumiso	5 g	RAPID	Step 1 2.0 % Step 2 0.1 %	Step 1 200 Step 2 110	7:45	39.4	2.79	
Rice Seasoning	3 g	RAPID	Step 1 2.0 % Step 2 0.01 %	Step 1 200 Step 2 110	3:35	3.1	83.87	
Boiled fish paste	5 g	RAPID	Step 1 1.0 % Step 2 0.01 %	Step 1 200 Step 2 105	21:30	73.8	0.14	
Sake lees	3 g	RAPID	Step 1 1.5 % Step 2 0.01 %	Step 1 200 Step 2 105	21:30	55.8	4.30	
alted rice malt	5 g	RAPID	Step 1 2.0 % Step 2 0.05 %	Step 1 200 Step 2 115	14:20	46.2	0.82	
oy sauce	5 g	RAPID	Step 1 1.0 % Step 2 0.01 %	Step 1 200 Step 2 105	10:40	68.2	0.19	
Miso	5 g	RAPID	Step 1 2.0 % Step 2 0.05 %	Step 1 200 Step 2 115	15:22	50.8	1.79	
Sardine dumplings	5 g	RAPID	Step 1 0.5 % Step 2 0.02 %	Step 1 200 Step 2 115	23:20	72.1	0.29	
Plastic (ABS pellet)	5 g	TIME	12 min	150	12:00	0.27	4.33	

Note 1: Measurement times, moisture ratios, and CV (%) values are aggregated from three data cycles. Note 2: The CV (%) is the standard deviation divided by the average value, multiplied by 100 to represent it as a percent.

Electronic Printers

FP-100/EP-110

Enhanced Support for ISO/GLP/GMP



· Enhanced Visibility for **OLED Display**

 Includes Functionality for Preventing **Date Alterations**

EP-110



EP-100/110 Shared Functionality

- Built-In Clock Date/time can be printed even for balances without a clock function
- Customized Printing In addition to weight measurement values, print items can be added to the end.
- Easy Communication Settings Includes functionality (automatic setting function) that automatically sets communication settings based on the given

Note: This function is disabled for ELB series models and MOC63u moisture analyzers.

Titles for measurement values can be customized for printing.

Compatible Balance Models AP, AU, AT-R, AT, U, TX, TXB, BX/BW-K, BL, and ELB series, and MOC63u moisture analyzers.

Note: The automatic setting function cannot be used with models that do not include the PRINT key, such as ELB series balances and MOC63u moisture analyzers.

Specifications

Model	EP-100	EP-110				
Display	_	OLED 128 × 64 Dot Matrix Display Easy-to-understand fluorescent dot matrix display				
Protected Date Setting	—	Password protectable (six-character)				
Printing	Method: 8-pin reciprod	ular paper (does not fade with age) cating impact dot matrix es/sec. Printer head life: 1 million lines . W1.7 × H2.6 mm				
Interface	USB B-Type female, RS	-232 (D-sub 9-pin male)				
Power Supply	AC adapter: Input 100 to 240 V AC, 50/60 Hz; Output 12 V DC/1500 mA Power consumption: 8 W (while printing) Standby power: 0.5 W (when not printing)					
Battery	_	1500 to 2500 mAh capacity rechargeable nickel- metal hydride (NiMH) batteries can be used (four AA cells). Note: Dry cell batteries cannot be used.				
Installation Environment	Temperature: 5 to 45 °	C; Humidity: 10 to 80 % No condensation				

Maintenance Parts

Description								
Recording Paper								
Labeling Paper Rolls								
Ink Ribbon								
AC Adapter								
Connection Cable								

EP-110 Function

Supports GLP/GMP Using Password Protection-**Based Date/Time Alteration Prevention**

Powered by Rechargeable Batteries

Eliminating the need for an AC adapter connection, the printer can be used as a portable device. It also means the printer can be used in locations without a power supply outlet, such as within a fume hood. Note: Dry cell batteries cannot be used (compatible with nickel metal hydride batteries).

Status Display with Enhanced Visibility for **OLED Display**

The OLED display makes it easier to determine the measurement mode-based status. The OLED display also ensures visibility even in dark locations.









(Printout Samples)

Manufacturer Information Shimadzu Corporation Nanufacturer Information Device Name Serial No. Sample Name (ID) Date Measurement Start Time AUW228 D23452456 Date: Start Time: 10.0000 g 10.0001 g 10.0002 g Measurement Values -

Normal Mode

Measurement End Time — Signature Field - Signature:

Shimadzu Corporation Model: 5/N: ID: D23452456 19.9996 g No.991 No.002 No.003 30.0021 g 10.0008 g 10.0006 g 0.0002 g 10.00070 g MAX= MIN-RNG= MEAN= SD-CV-0.00010 22126155 End Time Signature:

Statistical Calculation Mode

Output Items

Item	Symbol	Remarks
Title (Header)		Manufacturer information, device name, serial number (S/N),
		date, and measurement start time
Number of samples	N	
Total value	T	
Maximum value	MAX	
Minimum value	MIN	
Range	RNG	= MAX - MIN
Mean value	MEAN	= T / N
Standard deviation	SD	√ Σ(Xi-MEAN)²/(N-1)
Coefficient of variation	CV	(SD / MEAN x 100)%
Data suffix (footer)		Measurement end time and signature field



Attach Optional Kit for Use as a Specific Gravity Analyzer

When combined with an optional specific gravity measurement kit, balances can be used to measure specific gravity.


Operations are simplified by a text-based navigation function. By using sinkers, the specific gravity of liquid can be measured as well. This allows easily measuring the specific gravity of metals, rubbers, plastics, and other materials.



SMK-601 specific gravity measurement kit







First measure the in-air weight.



Then place it in the container filled with water, as instructed on the screen.



The specific gravity value is displayed using simple steps.

AP Series

		W Series						X Series			Y Series		
Model	AP225W	AP135W	AP125WD	AP225WD	AP124W	AP224W	AP324W	AP124X	AP224X	AP324X	AP124Y	AP224Y	AP324Y
Capacity	220 g	135 g	120 g / 52 g	220 g /102 g	120 g	220 g	320 g	120 g	220 g	320 g	120 g	220 g	320 g
Minimum Display	0.01	l mg	0.1 mg / 0.01 mg					0.1 mg					
Pan Size (mm)		Approx. ø91											
Dimensions	Approx. W21	Approx. W212 × D411 × H345 mm (incl. power supply unit) Approx. D212 × D367 × H345 mm											
Weight		Approx. 7.9 kg Appro					Approx	. 7.0 kg			А	pprox. 6.5 k	g
Required Power Supply		AC 100 V 270 mA 50/60 Hz											

Specific Gravity Measurement Kit

Model	SMK-601

Note: The optional liquid density sinker is required for liquid density measurements.

Optional Accessories
Description
Liquid Density Sinker
Petri Dish, Square

AT-R Series

Specific Gravity Analyzer



Measures a Variety of Gravity Values with the Immersion Method

Attach the optional SMK-401 Specific Gravity Measurement Kit to a balance in the AU series, and set the balance to specific gravity measurement mode. You can then use the balance as a specific gravity analyzer, capable of automatically calculating and displaying specific gravity values.

Liquid density can also be measured by using an optional sinker.

Various balances are available, including a semi-micro (0.01 mg) model. Choose the model best suited to the sample amount and required precision in your application.

Two kinds of weighing pans as standard.















AU Series

	AUW-D	AUW-D Series		AUW Series			AUX Series	AUY Series		
Model name	AUW220D	AUW120D	AUW320	AUW220	AUW120	AUX320	AUX220	AUX120	AUY220	AUY120
Capacity	220 g/82 g	120 g/42 g	320 g	220 g	120 g	320 g	220 g	120 g	220 g	120 g
Minimum Display	0.1 mg/	0.1 mg/0.01 mg		0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg
Repeatability	0.1 mg/0.05 mg	0.1 mg/0.02 mg	0.15 mg	0.1 mg	0.1 mg	0.15 mg	0.1 mg	0.1 mg	0.1 mg	0.1 mg
Pan Size (mm)		Approx. 80 dia.								
Body Dimensions		Approx. W217 × D356 × H338 mm								
Weight		Approx. 7 kg								

Specific Gravity Measurement Kit

Description	Description
SMK-401	Liquid Density Sinker
	Petri Dish, Square

O	p	tie	or	ıal	Α	CC	e	SS	o	rı	es



Measures a Variety of Specific Gravity Values with the Immersion Method

Attach the optional SMK-501 Specific Gravity Measurement Kit to a balance in the AT-R series, and set the balance to specific gravity measurement mode. You can then use the balance as a specific gravity analyzer, capable of automatically calculating and displaying specific gravity values.

Liquid density can also be measured by using an optional sinker.

Various balances are available. Choose the model best suited to the sample amount and required precision in your application.



SMK-501 Specific Gravity Measurement Kit







AT-R Series

Model	ATX324R	ATX224R	ATX124R	ATX84R	ATY324R	ATY224R	ATY124R	ATY64R		
Capacity	320 g	220 g	120 g	82 g	320 g	220 g	120 g	62 g		
Minimum Display		0.1 mg								
Pan Size (mm)		Approx. 91 dia.								
Dimensions		Approx. W213 × D356 × H338 mm								
Weight	Weight Approx. 6.2 kg Approx. 6.0				κ. 6.0 kg					

Specific Gravity Measurement Kit

	Description	
SMK-501		

Description	
Liquid Density Sinker	
Petri Dish, Square	

Specific Gravity Analyzer



Measures a Variety of Gravity Values with the Immersion Method

Attach the optional SMK-101A/102 Specific Gravity Measurement Kit to a balance in the UP series, and set the balance to specific gravity measurement mode. You can then use the balance as a specific gravity analyzer, capable of automatically calculating and displaying specific gravity values.

Liquid density can also be measured by using an optional sinker.

Various balances are available. Choose the model best suited to the sample amount and required precision in your application.

The large submersible pan makes it easy to measure bulky samples.





ι	JP Series Balances (lar	ge pan type))					Models with	built-in calibra	tion weights	
	Model	UP2202Y	UP2202Y UP4202Y UP6202Y UP4201Y UP8201Y UP2202X UP4202X UP6202X UP4201X UP								UP8201X
_	Capacity	2200 g	4200 g	6200 g	4200 g	8200 g	2200 g	4200 g	6200 g	4200 g	8200 g
-	Minimum Display		0.01 g		0.	1 g		0.01 g 0.1 g			
	Pan Size (mm)		Α	pprox. 170 x 18	30			А	pprox. 170 x 18	30	

UP Series Balances (small pan type)									Mod	dels with b	uilt-in calib	oration weig	ghts	
Model	UP223Y	UP423Y	UP623Y	UP823Y	UP1023Y	UP422Y	UP822Y	UP223X	UP423X	UP623X	UP823X	UP1023X	UP422X	UP822X
Capacity		420 g	620 g	820 g	1020 g	420 g	820 g		420 g	620 g	820 g	1020 g	420 g	820 g
Minimum Display			0.00	01 g		0.0)1 g			0.0	01 g		0.0	11 g
Pan Size (mm)	1/		Approx. 108 × 105								Approx.	108 × 105		

Specific Gravity Measurement Kit

Model	SMK-101A for large pan*1*2
	SMK-102 for small pan*1*3

Optional Accessories

Description
Liquid Density Sinker for SMK-101A/102

- *1 The optional liquid density sinker is required for liquid density measurements.
- *3 For UP-X/UP-Y series small-pan (170 × 180 mm) types. The actual capacity is 100 g less than the capacity of the balance.

 *3 For UP-X/UP-Y series small-pan (108 × 105 mm) types. The actual capacity is 290 g less than the capacity of the balance. Cannot be attached to the UP223X/UP223Y.

In addition to the above-mentioned, balances with the 📴 mark are equipped with a specific gravity calculation function, so they can be used for specific gravity measurement.

UW/UX series

Measures a Variety of Specific Gravity Values with the Immersion Method

Attach the optional SMK-101/102 Specific Gravity Measurement Kit to a balance in the UW/UX series, and set the balance to specific gravity measurement mode. You can then use the balance as a specific gravity analyzer, capable of automatically calculating and displaying specific gravity values.

Liquid density can also be measured by using an optional sinker.

Various balances are available. Choose the model best suited to the sample amount and required precision in your application.

The large submersible pan makes it easy to measure bulky samples.





UW/UX Series + SMK-101

.

UW/UX Series Balan	ices (large pa	n type)				Models with built-in calibration weights					
Model	UX2200H	UX4200H			UX8200S	UW2200H UW4200H		UW6200H	UW4200S	UW8200S	
Capacity	2200 g	4200 g	6200 g	4200 g	8200 g	2200 g	4200 g	6200 g	4200 g	8200 g	
Minimum Display		0.01 g 0.1 g					0.01 g 0.1 g				
Pan Size (mm)		A	pprox. 170 × 18	30			А	pprox. 170 × 18	30		

UW/UX Series Balan	ices (smal	l pan typ	e)					Models with built-in calibration weights						
Model	UX220H	UX420H	UX620H	UX420S	UX820S	UX820H	UX1020H	UW220H	UW420H	UW620H	UW420S	UW820S	UW820H	UW1020H
Capacity		420 g	620 g	420 g	820 g	820 g	1020 g		420 g	620 g	420 g	820 g	820 g	1020 g
Minimum Display		0.00	0.001 g 0.01 g 0.001 g					0.001 g 0.01 g 0.001 g						
Pan Size (mm)				Approx.	108 × 105						Approx.	108 × 105		

Specific Gravity Measurement Kit

Model	SMK-101 for large pan ^{*1*2}
	SMK-102 for small pan*1*3

Optional Accessories

Description
Liquid Density Sinker for SMK-101/102

- *1 The optional liquid density sinker is required for liquid density measurements.
- *2 For UW/UX series large-pan (170 × 180 mm) types. The actual capacity is 100 g less than the capacity of the balance.
 *3 For UW/UX series small-pan (108 × 105 mm) types. The actual capacity is 290 g less than the capacity of the balance. Cannot be attached to the UW/UX 220H.

In addition to the above-mentioned, balances with the 🛅 mark are equipped with a specific gravity calculation function, so they can be used for specific gravity measurement.

Attach an optional animal bucket to a UP series

balance, and set the unit to animal mode. The balance can now be used as a user-friendly animal balance.

Animal Balances

F

Animal Balances



Quick, Stable Measurements of Animal Weight







Bucket for small animals

Deep round bucket

Rectangular bucket



Clock-CAL

This automatically calibrates the balance at pre-specified times (such as before starting work, during lunch, or after work hours).



Internal Calibration

The balance has built-in motor-driven calibration weights. Sensitivity can be calibrated whenever needed with a single key press.



Built-in Animal Measurement Mode

- When the animal is unloaded, residual weight from excretions and other materials is automatically subtracted and the display is set to zero. The next animal can be loaded without pressing the TARE button, which increases efficiency
- Thanks to the specially developed animal measurement software, the weight of moving animals is measured quickly and stably.

UP-X Series

















































UP-X/UP-Y Series (balance)

A4 - 4 - 1		S	tandard mode	ls		Models with built-in calibration weights					
Model	UP2202Y	UP4202Y	UP6202Y	UP4201Y	UP8201Y	UP2202X	UP4202X	UP6202X	UP4201X	UP8201X	
Capacity	2200 g	4200 g	6200 g	4200 g	8200 g	2200 g	4200 g	6200 g	4200 g	8200 g	
Minimum Display	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g	0.01 g	0.01 g	0.01 g	0.1 g	0.1 g	

Bucket

Small Animal Bucket	Shape: round / Size: bottom 110 dia. × top 200 dia. × height 130 (mm)
Deep Round Bucket	Shape: round / Size: bottom 155 dia. × top 195 dia. × height 200 (mm)
Rectangular Bucket *1	Shape: rectangular / Size: bottom 250 × 210; top 290 × 250; height 150 (mm)

^{*1} The rectangular bucket can only be attached to the UP8201X and UP8201Y. Note: Can also be used with the UW/UX Series.

Three movement levels can be selected corresponding to the animal movement.

Animals can be measured whether they are docile or extremely active.

When the animal is loaded and the stability mark is displayed, the weight is output automatically. Needless operation is eliminated to increase efficiency.

When the animal is unloaded, residual weight from excretions and other materials is automatically subtracted and the display is set to zero.

The next animal can be loaded without pressing the TARE button, which increases efficiency.

Quick, Stable Measurements of Animal Weight

BW-K/BX-K series

Attach an optional animal bucket to a BW-K/BX-K series balance, and set the unit to animal mode. The balance can now be used as a user-friendly animal balance.



Built-in Animal Measurement Mode

- Models with a range of capacities are available. Ideal for medium weight measurements of rabbits and small dogs.
- Thanks to the specially developed animal measurement software, the weight of moving animals is measured quickly and stably.
- When the animal is unloaded, residual weight from excretions and other materials is automatically subtracted and the display is set to zero. The next animal can be loaded without pressing the TARE button, which increases efficiency.





Medium bucket set

Small bucket set

BW-K Series





































Model Models with built-in calibration weights						Standard models						
Model	BW12KH	BW22KH	BW32KH	BW32KS	BW52KS	BX12KH	BX22KH	BX32KH	BX32KS	BX52KS		
Capacity*1 *2	12 kg	22 kg	32 kg	32 kg	52 kg	12 kg	22 kg	32 kg	32 kg	52 kg		
Minimum Display	0.1 g	0.1 g	0.1 g	1 g	1 g	0.1 g	0.1 g	0.1 g	1 g	1 g		

Bucket

Small Bucket (mainly suited to rabbits)	Shape: rectangular / Size: bottom 305 × 215; top 335 × 245; height 215 (mm)
Medium Bucket (mainly suited to small dogs)*3	Shape: rectangular / Size: bottom 335 × 245: top 445 × 295; height 345 (mm)

- *1 When an animal bucket is attached, the capacity will be reduced about 2 kg from the value indicated.
 *2 When an animal bucket is attached, the capacity will be reduced about 6 kg from the value indicated.
- *3 The bucket cannot be attached to the BW12KH or BX12KH.

Shared Options for the UP-X/UP-Y & UW/UX & BW-K/BX-K


Description	
Electronic Printer EP-100	
Electronic Printer EP-110	
RS-232C Cable (1.5 m)	
USB–Serial Conversion Kit	



LabSolutions Balance



Integrate Analysis Data Acquired from Balances to Analytical Network Data System Compliant with PIC/S GMP and ER/RS Regulations

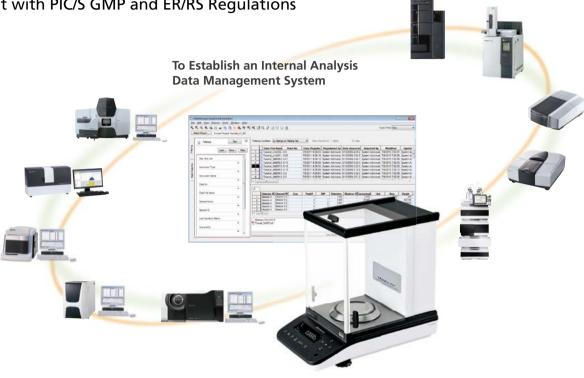

Improves Operational Efficiency and Data Reliability

- Eliminate manual entry; all the weighing data are saved automatically in a safe database without transcription mistakes.
- Reports appropriate for weighing methods, such as the mass variation test, drying weight
 loss test and particle size test, can be created automatically after the measurement. In
 addition, customized reports featuring such information as system conformance, content
 uniformity and elution tests together with the analysis results obtained by HPLC, etc. can be
 created.




Main Window of LabSolutions Balance

Integrated Management of Analytical Data on Network System Using LabSolutions




Compliant with the Latest Data Integrity Guidance (U.S. FDA 21 CFR Part 11)

- Weighing results can be automatically saved in the database together with other information, including sample ID, operator name, operation date and series number of instrument used. This enables quick data searching based on sample information.
- It allows setting up user authority to ensure only the authorized user can create a template for weighing.
- It prevents improper manipulation or unintended overwriting and deletion of data. In addition, measurement results and all the operation histories and reasons will be saved in the database as log files.

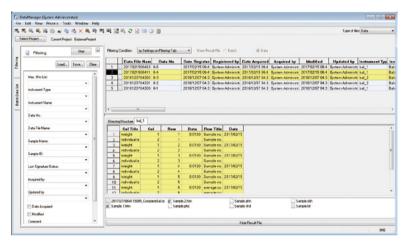

LabSolutions Data Manager

Integrated Report Creation Function Combines Analysis Results from HPLC and Weighing Results from Balance

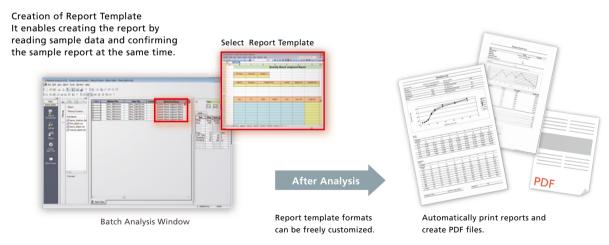

Note: Multi-data report creation (optional) is necessary to use this function.

Specifications

OS	Windows® 7 Professional SP1 (32 bit/64 bit), Windows® 10 Pro
Compatible Instruments	Shimadzu AP, AU, AT-R, AT, UP and UW/UX series
Other Functions	Controls up to 2 balance units, generation of PDF files, interface supporting linkage to LIMS system (option)

Accessories for Shimadzu Balances

		AP	AUW-D AUW AUX AUY	ATX-R ATY-R	ATX ATY	UP-X UP-Y	UW UX	тх	ТХВ	BL	ELB	BW-K BX-K	MOC- 120H	MOC63u
EP-100	3													
EP-110		/	1	1	✓	/	√	/	1	✓	•	/		1
Printer for MOC	-120H												1	
IFB-102A-UNC		Built-in	Built-in	Built-in	1	Built-in	Built-in	Built-in	Built-in	1	1	Built-in	Built-in	Built-in
I/O-RS cable		Built-in	Built-in	Built-in	1	Built-in	Built-in	Built-in	Built-in	1	1	Built-in	Built-in	Built-in
AKB-301 Application keyb			1			1	1					1		
Windbreak WB0 for UW/UX small-						1	1							
Large windbrea for UW/UX Series						1	1							
USB conversion with RS-232C ca			1		1	1	1	1	1	✓	1	1	*1	1
Foot switch	for print FSB-102PK		1			1	1					1		
	for TARE FSB-102TK		1			1	1					1		
	SMK-101A					1								
	SMK-101						1							
	SMK-102					1	1							
measurement	SMK-201 for ELB large-pan model										1			
kit	SMK-401		1											
	SMK-501			1										
	SMK-601	1												

Optional accessories list


Balances	Optional accessories						
AP Series	Static Electricity Remover STABLO-AP Ionizer						
	Electronic Printer EP-100 / EP-110						
	Label Roll Paper for EP-100/110 (10 Rolls)						
	Specific Gravity Measurement Kit SMK-601						
	Display Protective Cover (Set of 5)						
	USB Cable						
	RS-232 Cable						
	AC Adapter (Standard Accessory)						
	Internal Windbreak Plate						
	RS–IO Interface Cable						
	AP Holder (Standard Accessory for AP225W)						
AUW-D /	Electronic Printer EP-100 / EP-110						
AUW / AUX /	Foot Switch FSB-102TK (For taring)						
AUY Series	Foot Switch FSB-102PK (For printing)						
	Specific Gravity Measurement Kit SMK-401						
	Application Keyboard AKB-301						
	RS-232C Cable, for IBM PC/AT Compatibles (25P–9P, Null modem, 1.5 m)						
	In-use Protective Cover (5 pcs)						
ATX-R / ATY-R	Static Electricity Remover STABLO-AP Ionizer						
Series	Electronic Printer EP-100 / EP-110						
	USB Cable Set						
	SMK-501 Specific Gravity Measurement Kit						
	AP Holder						
	Protective Cover (5 pc set)						
	AC Adapter (provided as standard with the main unit)						
ATX / ATY	Electronic Printer EP-100 / EP-110						
Series	IFB-102A-UNC						
	USB Conversion Kit						
	In-use Protective Cover (5 pcs)						
	I/O–RS Cable						
TX / TW /	Electronic Printer EP-100 / EP-110						
TXB / TXC /	In-use Protective Cover (5 pcs)						
TWC Series	RS-232C Cable						
BL Series	Electronic Printer EP-100 / EP-110						
	In-use Protective Cover (5 pcs)						
	Simple Windbreak						
	Lid for Simple Windbreak						
	IFB-102A-UNC						
ELB Series	Electronic Printer EP-100 / EP-110						
	RS-232C Interface IFB-102A-UNC						
	In-use Protective Cover (5 pcs)						
	Specific Gravity Measurement Kit SMK-201 (Cannot be used with small-pan models)						
BW-K / BX-K	Electronic Printer EP-100 / EP-110						
Series	RS-232C Interface IFB-102A (for multiple connections)						
	Foot Switch FSB-102PK (For printing)						
	Application Keyboard AKB-301						

Balances	Optional accessories
UP Series	Static Electricity Remover STABLO-AP Ionizer
	Electronic Printer EP-100 / EP-110
	RS-232C Cable 25P–9P (1.5 m)
	USB–Serial Replacement Kit
	Application Keyboard AKB-301
	Windbreak Set *1
	Windbreak Set (for large pan) *2
	Glass Windbreak WBC-102
	Large Size Windbreak WBC-502
	In-use Protective Cover (3 pcs) (For Large-Pan Models with 0.01 g Min. Display Value)
	In-use Protective Cover (5 pcs) (For Large-Pan Models with 0.1 g Min. Display Value)
	In-use Protective Cover (5 pcs) (For Small-Pan Model)
	In-use Protective Cover (5 pcs) (For Display and Key Part)
	Animal Bucket Set (for Large-Pan Models with 0.01 g Minimum Display Value)
	Animal Bucket Set (for Large-Pan Models with 0.1 g Minimum Display Value)
	Specific Gravity Measurement Kit SMK-101A (For Large-Pan Model) (Up to approximately 2 kg for weighing capacity)
	Specific Gravity Measurement Kit SMK-102 (For Small-Pan Model)
	Remote Display RDB-201
	Remote Display RDB-202
	Relay Output Interface IFB-RY1
	RY1 Connection Cable
	AC Adapter *3
UW / UX Series	Electronic Printer EP-100 / EP-110
	RS-232C Interface IFB-102A (for multiple connections)
	Small Size Windbreak (for models with capacity of 300 to 620 g only) (Std Acc. for models with readability of 1 mg)
	Glass Windbreak (for models with capacity of 220 to 820 g only)
	Large Size Windbreak (for all models)
	Specific Gravity Measurement Kit SMK-101 (for models with capacity of 2200 g and up only)
	Specific Gravity Measurement Kit SMK-102 (for models with capacity of 420 to 820 g only)
	In-use Protective Cover (5 pcs)
	Foot Switch FSB-102PK (For printing)
	Foot Switch FSB-102TK (For taring)
	RS-232C Cable, for IBM PC/AT Compatibles (25P–9P, Null modem, 1.5 m)
	RS-232C Cable, for multiple connections (25P–25P, Null modem, 1.5 m)
	Application Keyboard AKB-301
	Remote Display Unit RDB-201 with operation keys
	Remote Display Unit RDB-202
	Angle Adjuster and Wall Hook for Remote Display
	Stand for Remote Display (1-m high)
MOC63u	Electronic Printer EP-100 / EP-110
	In-use Protection Cover for Display (5 pcs)
	Aluminum Sheet
	Fiberglass Sheet
	Temperature Calibration Kit
	Sample Pan (SUS)
	RS-232C Cable
	USB Connection Cable
	Halogen Heater for Replacement


- *1 Included standard with small-pan models with 0.001 g minimum display value.
 *2 Included standard with large-pan models with 0.01 g minimum display value.
 *3 Included standard with main unit.

Physical Dimensions


AP Series

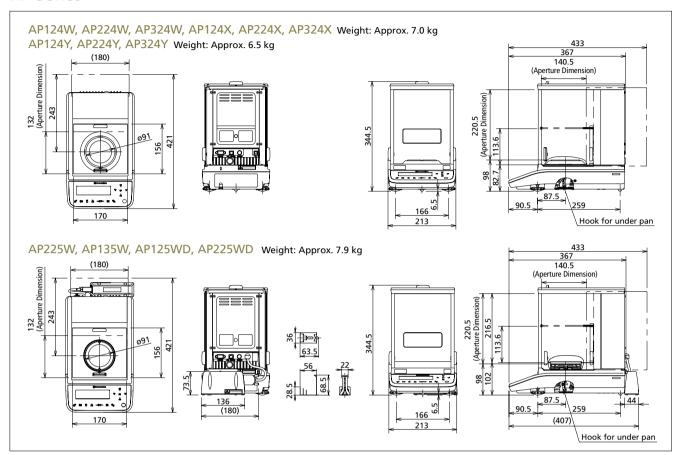


AUW-D/AUW/AUX/AUY Series

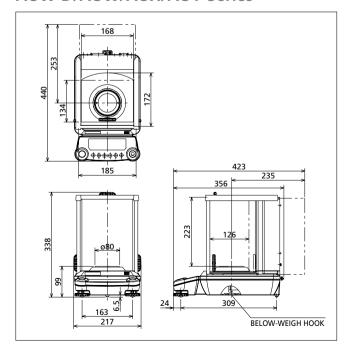


AT-R and ATX/ATY Series

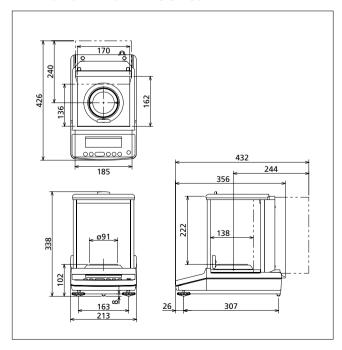

UP and UW/UX Series

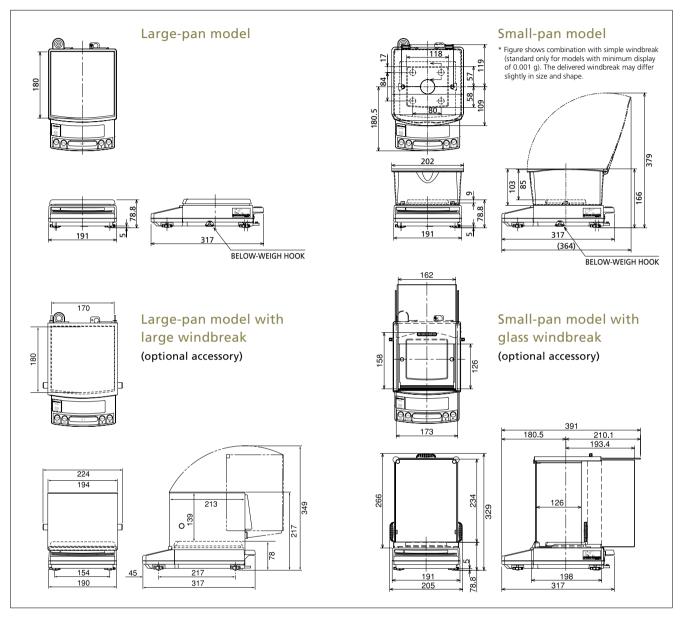


Below-weigh Hook

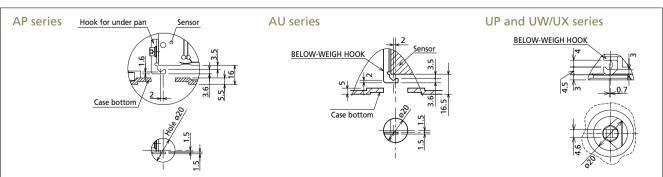


Physical Dimensions


TW/TX/TXB/TWC/TXC Series

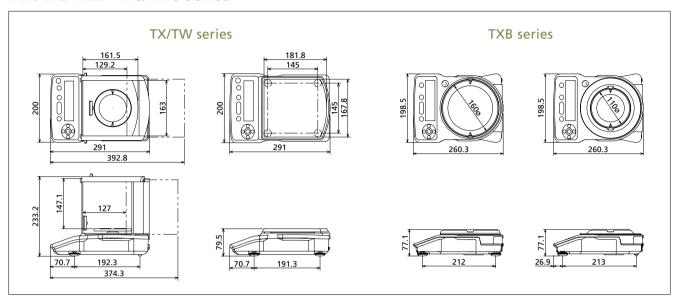


BL Series

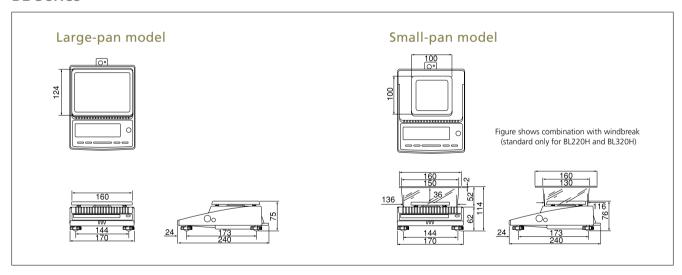


BW-K/BX-K Series

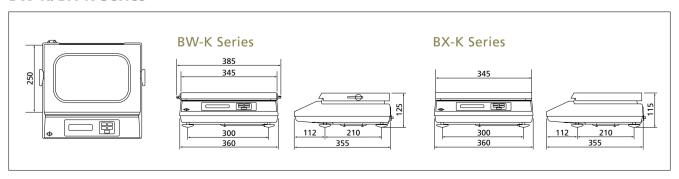


ELB Series

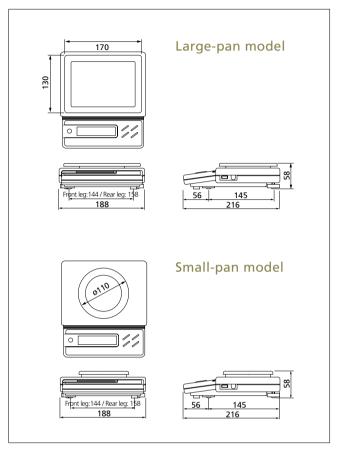


EP-100/EP-110

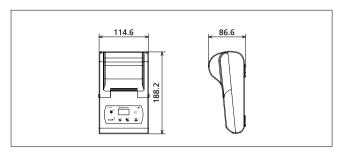


STABLO-AP

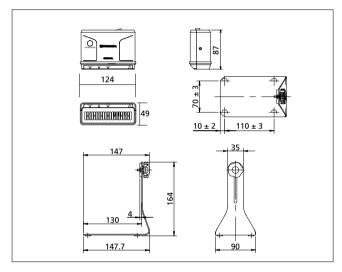

MOC63u

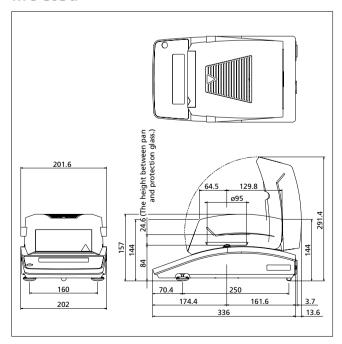

MOC-120H

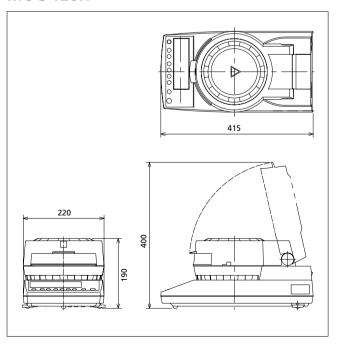

Shimadzu Electronic Balances Demonstration Movies





https://www.youtube.com/playlist? list=PLCPY11zjvhZPmTi_xW1oGJeSuI-YR6qaV

UniBloc, LabSolutions, STABLO and eco logo are trademarks of Shimadzu Corporation.
Windows and Excel are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.



Shimadzu Corporation www.shimadzu.com/an/

For Research Use Only. Not for use in diagnostic procedures.
This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

products in your country.

Company names, products/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation, its subsidiaries or its affiliates, whether or not they are used with trademark symbol "TM" or "®".

Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services, whether or not they are used with trademark symbol "TM" or "®".

Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The contents of this publication are provided to you "as is" without warranty of any kind, and are subject to change without notice. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication.